

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/28/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:04
INTERNAL STANDARD	VERIFIED	18:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:05
BLANK TEST	0.00	18:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:06
BLANK TEST	0.00	18:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:07
BLANK TEST	0.00	18:08

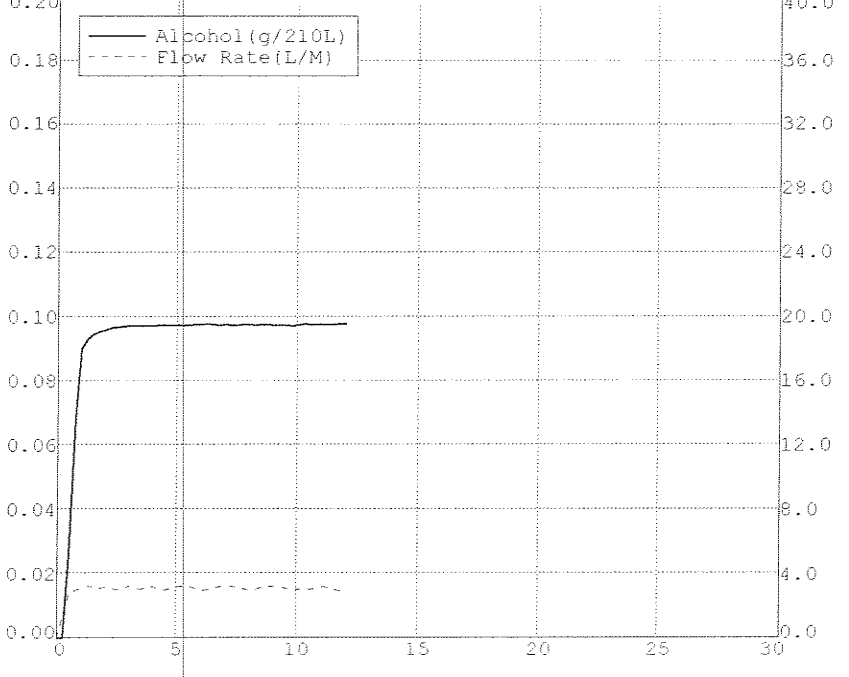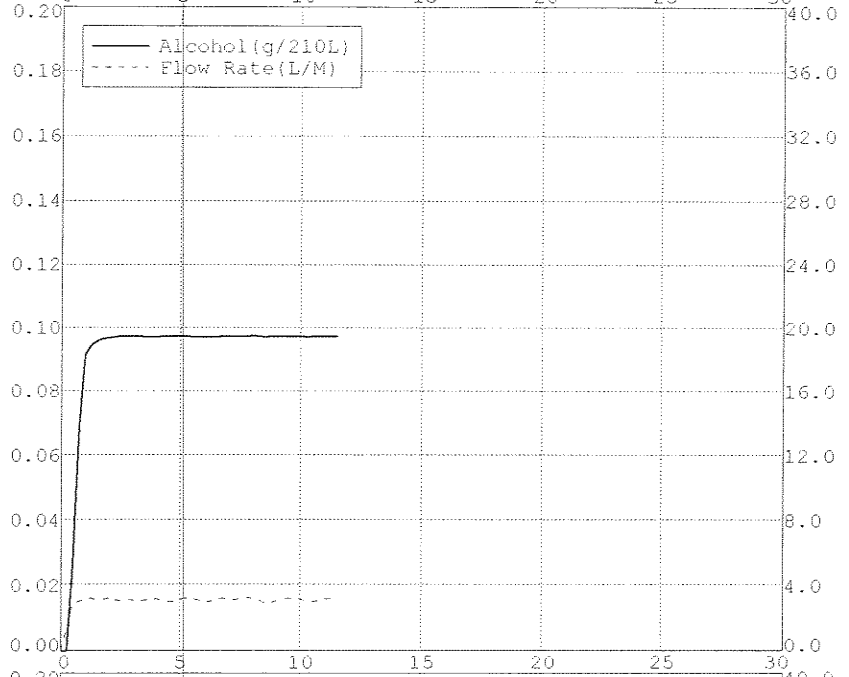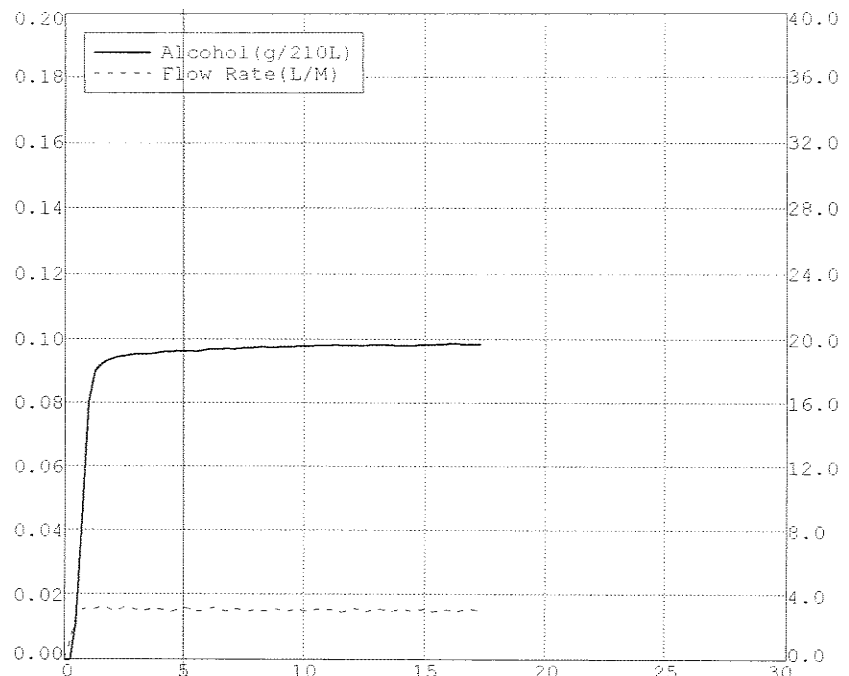

Signature
#241