

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/08/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:38
INTERNAL STANDARD	VERIFIED	17:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:39
BLANK TEST	0.00	17:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:40
BLANK TEST	0.00	17:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:41
BLANK TEST	0.00	17:42

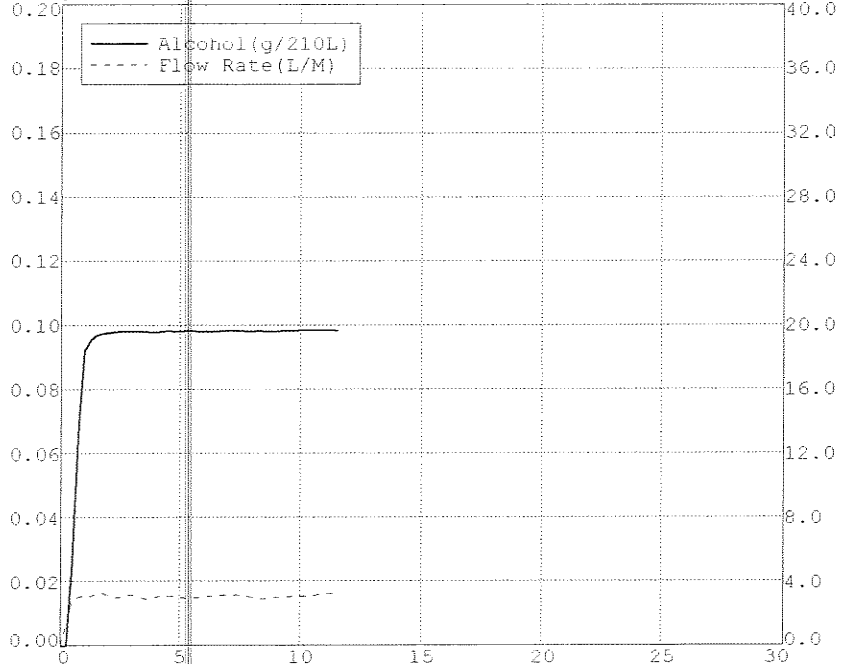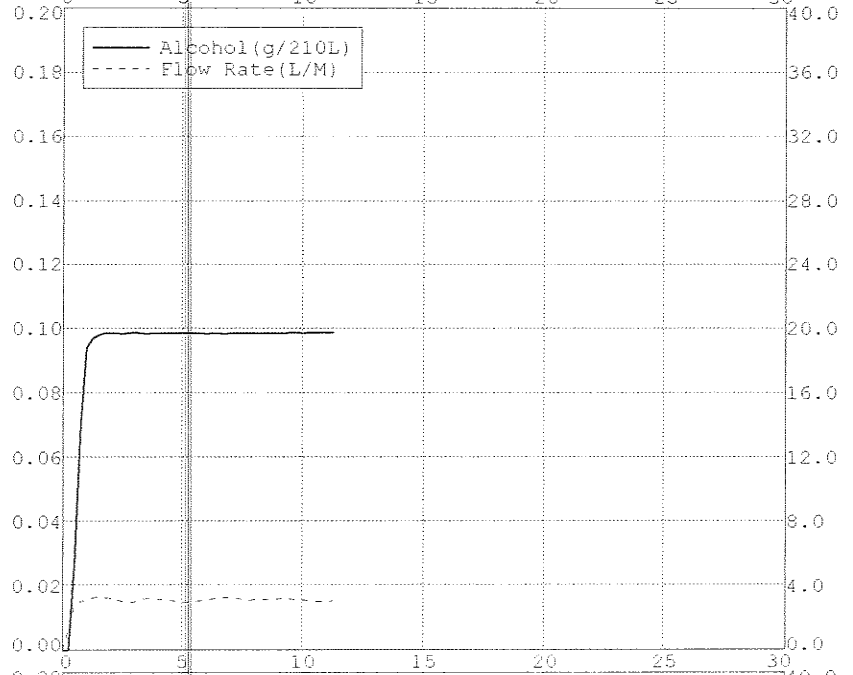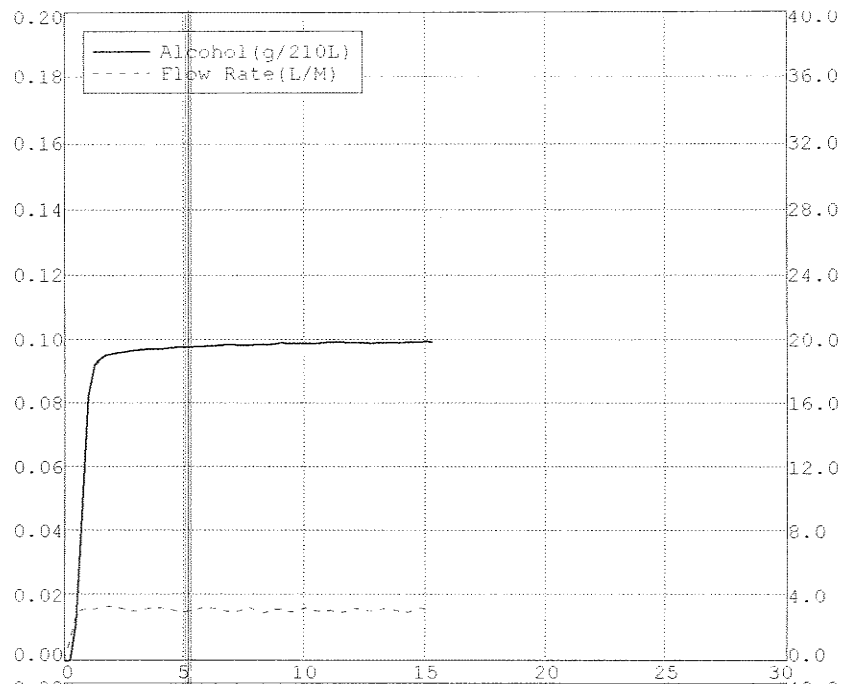

*Chl-B. [Signature] #245*