

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 11/25/2020

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:58
INTERNAL STANDARD	VERIFIED	16:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:59
BLANK TEST	0.00	17:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:00
BLANK TEST	0.00	17:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:01
BLANK TEST	0.00	17:02

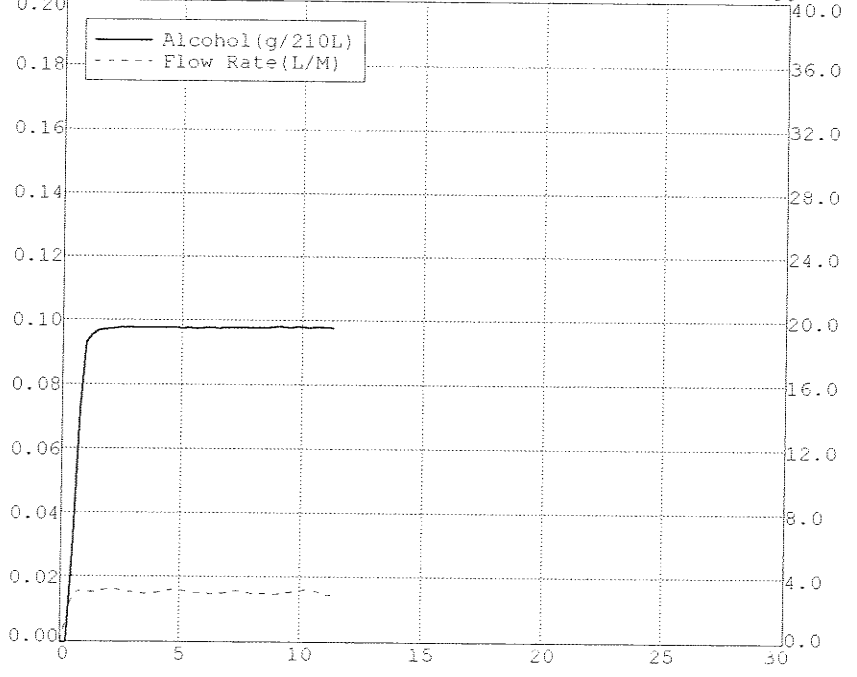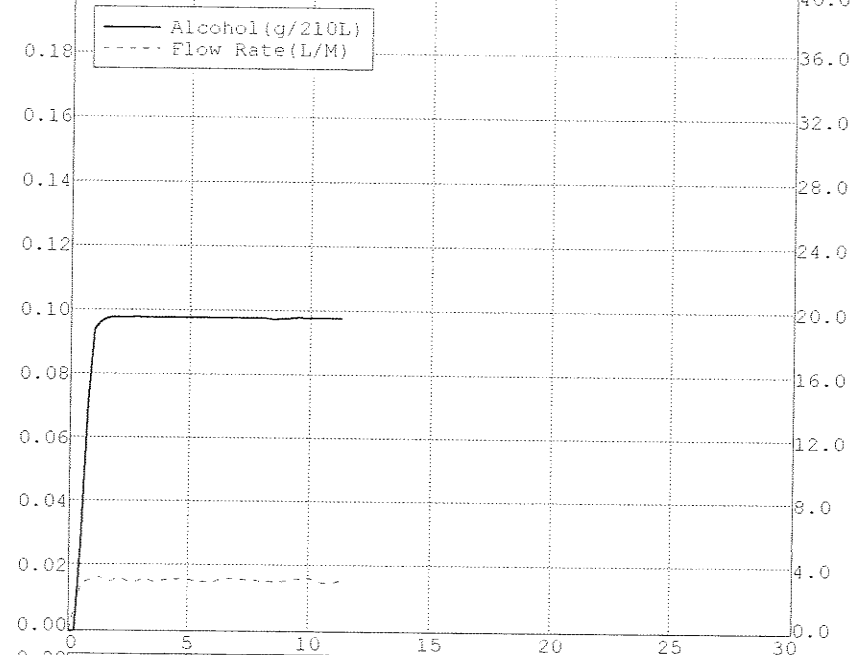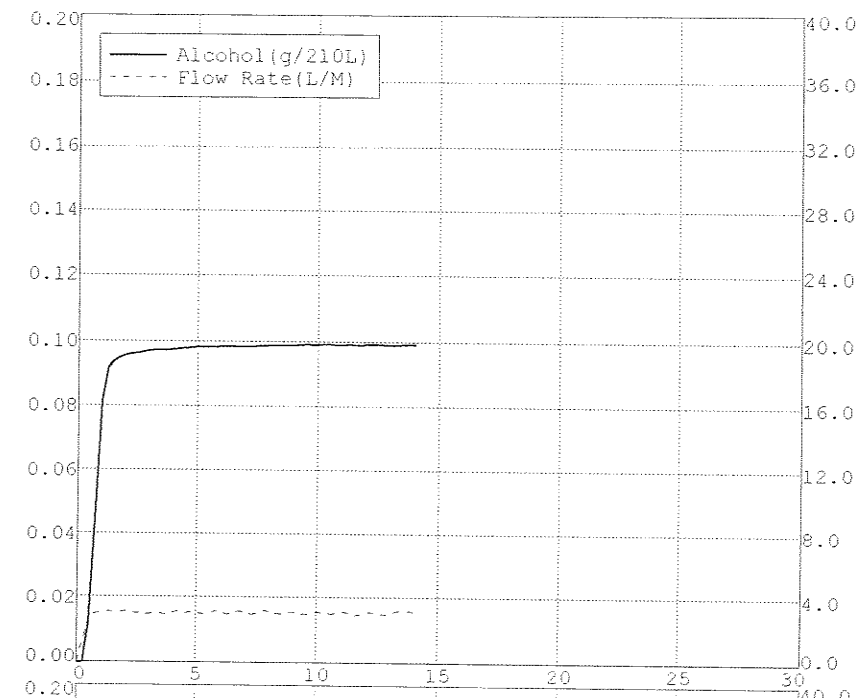

*Sgt. C. B. Geisler #221*