

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/06/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:31
INTERNAL STANDARD	VERIFIED	17:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:31
BLANK TEST	0.00	17:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:33
BLANK TEST	0.00	17:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:34
BLANK TEST	0.00	17:35

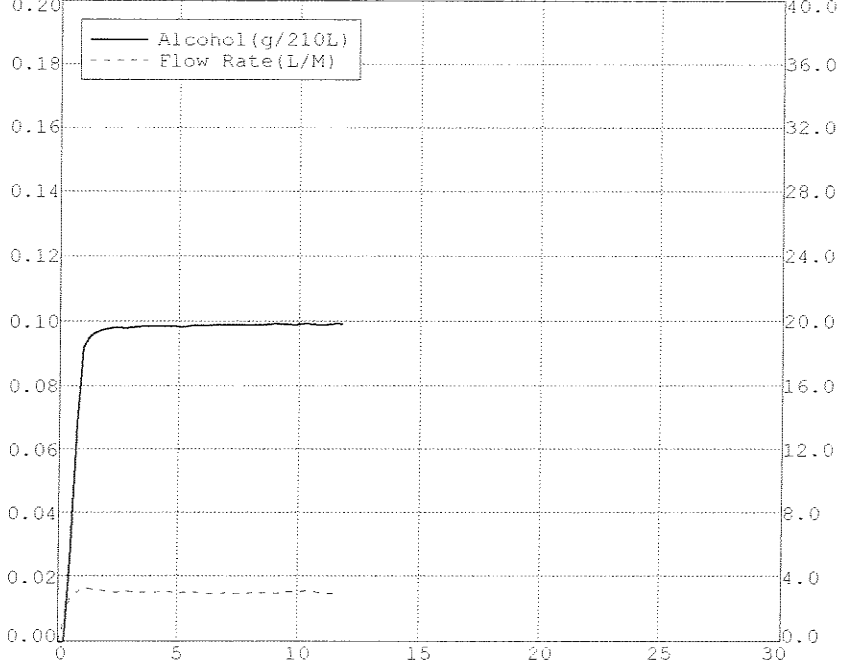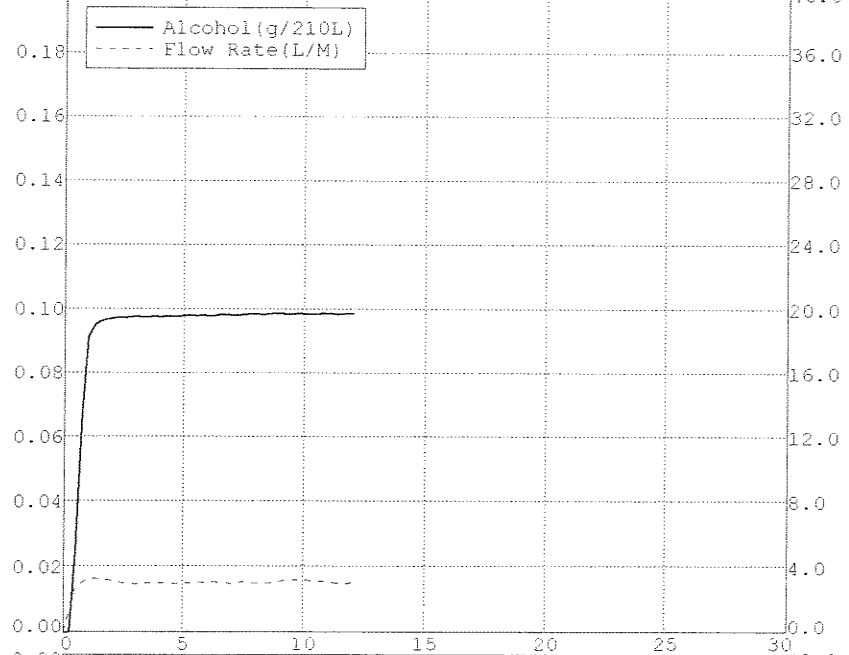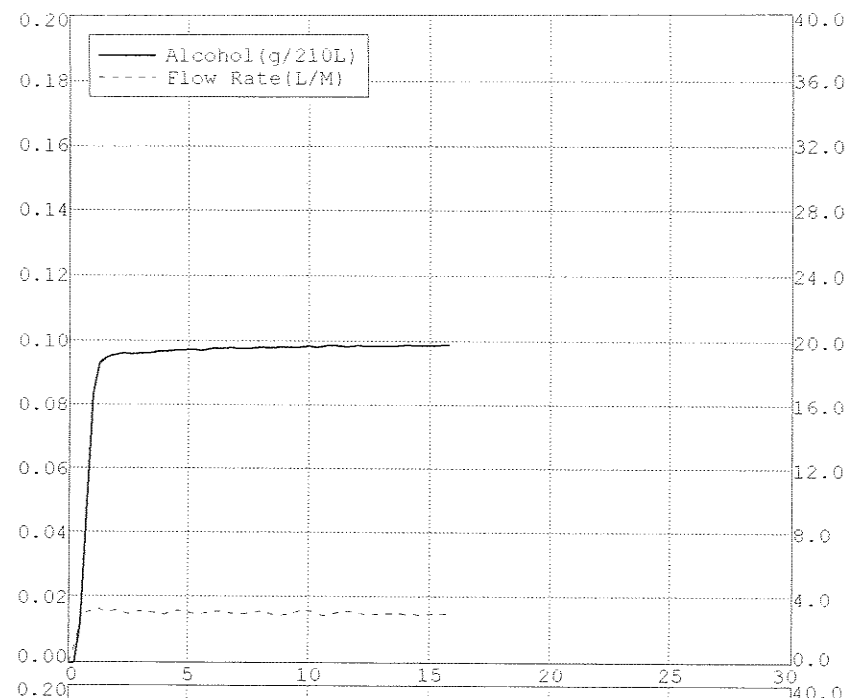

Sgt. C.B. Geisler #215