

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 12/14/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:31
INTERNAL STANDARD	VERIFIED	16:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:32
BLANK TEST	0.00	16:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:33
BLANK TEST	0.00	16:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:34
BLANK TEST	0.00	16:35

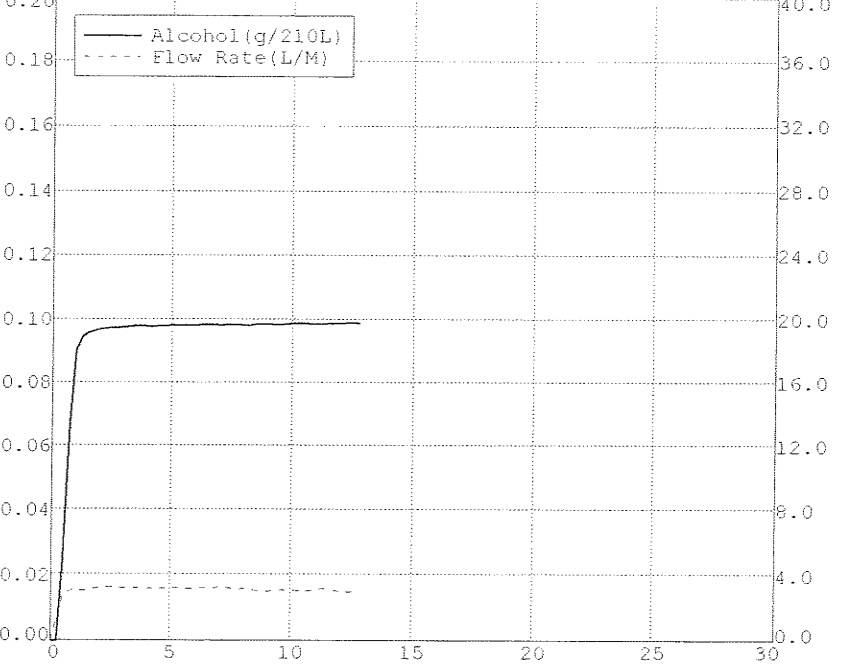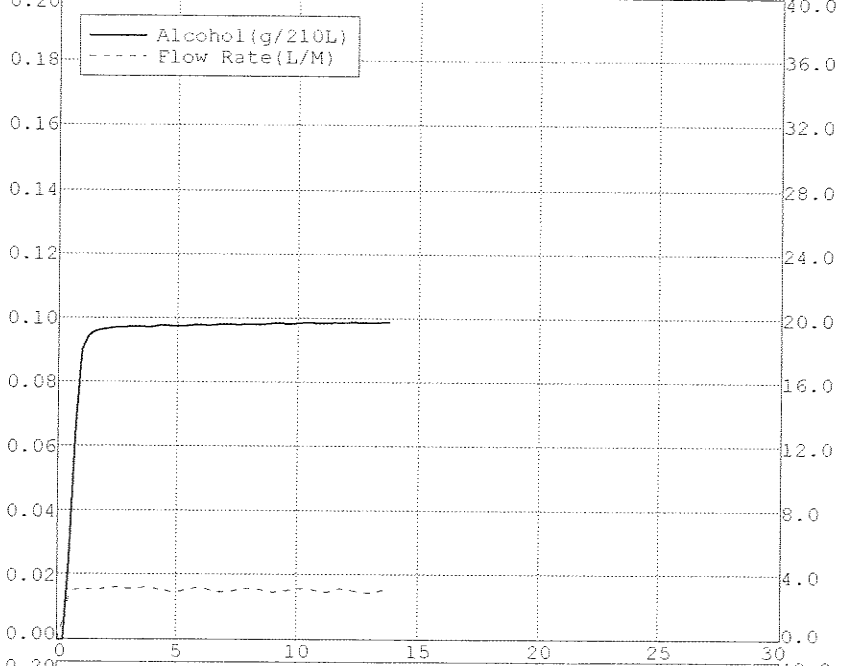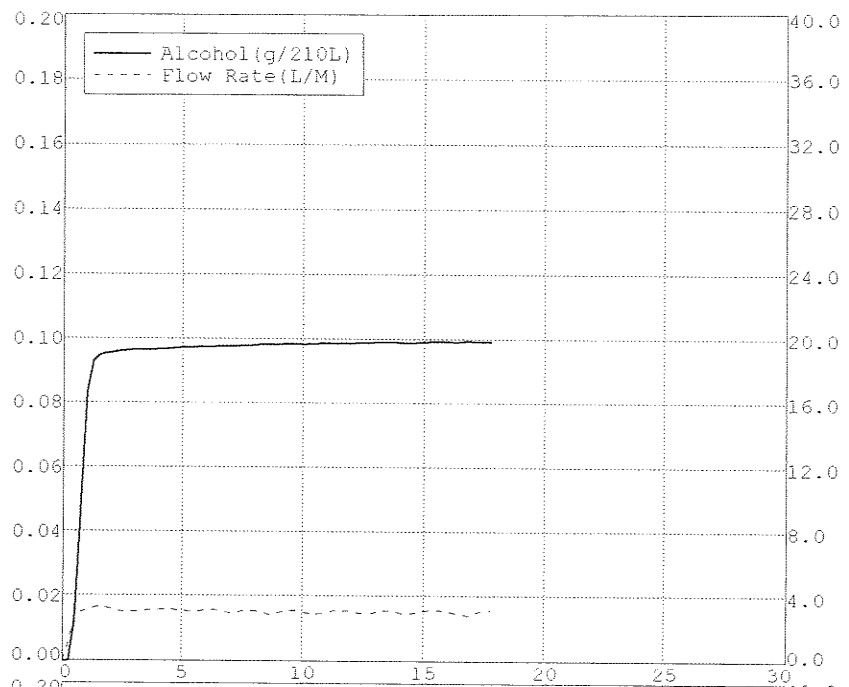

*Handwritten signature and initials* #248