

SUPERVISOR TEST



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/20/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20430

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 15:32 |
| INTERNAL STANDARD | VERIFIED | 15:32 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 15:32 |
| BLANK TEST | 0.00 | 15:33 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 15:34 |
| BLANK TEST | 0.00 | 15:35 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 15:35 |
| BLANK TEST | 0.00 | 15:36 |

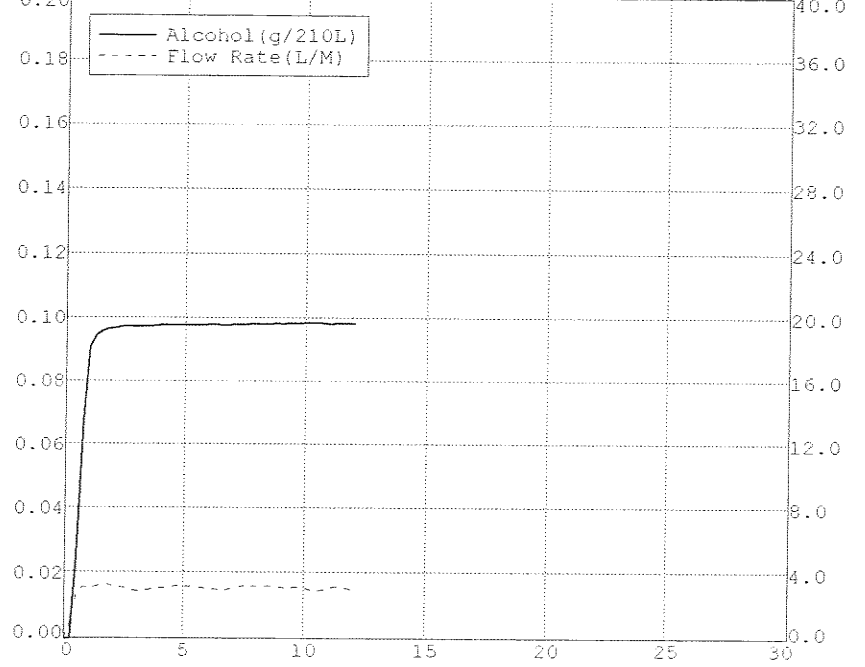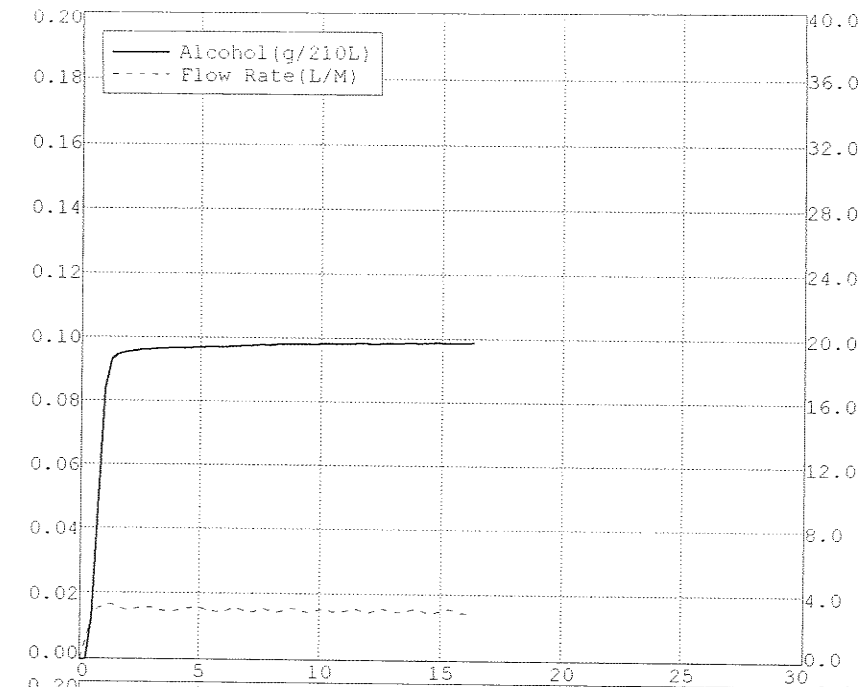

Ch. B. Geisler #241