

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 01/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:32
INTERNAL STANDARD	VERIFIED	18:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:32
BLANK TEST	0.00	18:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:33
BLANK TEST	0.00	18:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:34
BLANK TEST	0.00	18:35

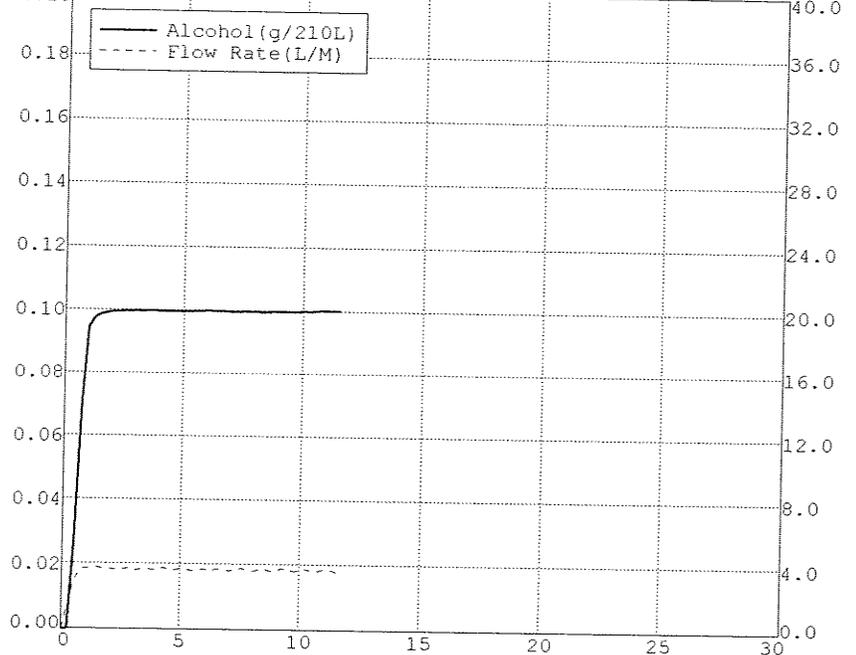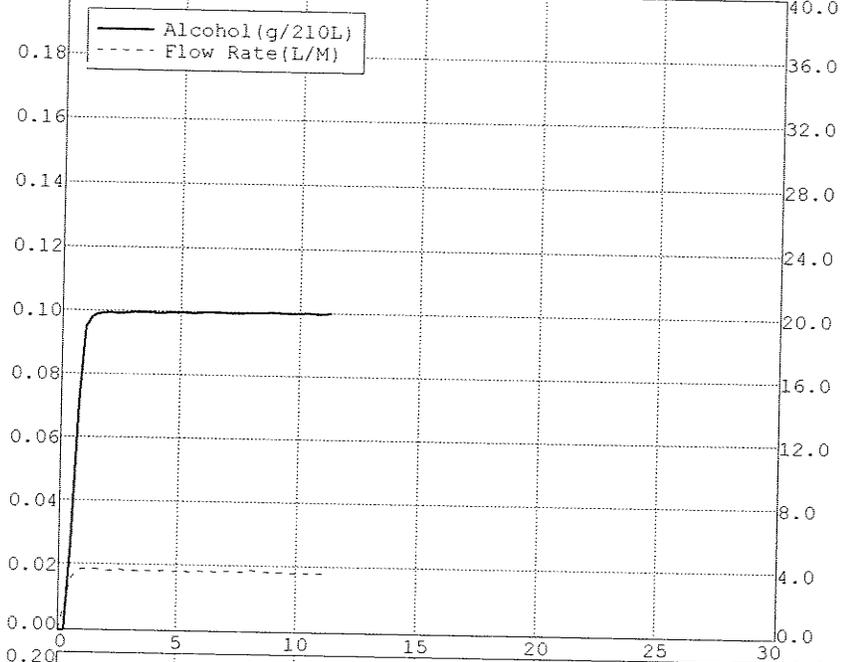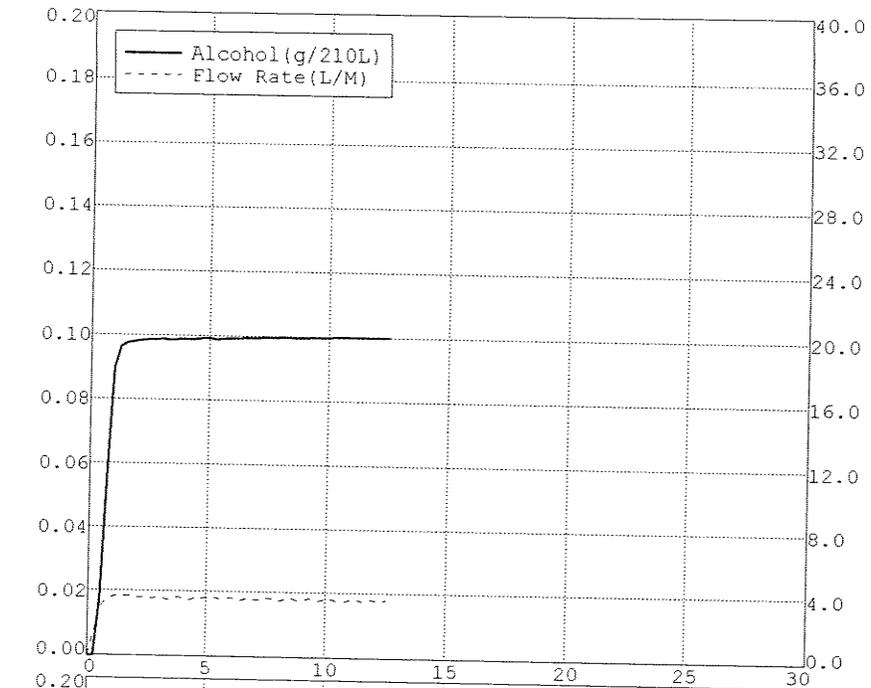

Charles B. Geisler #2115