

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 01/13/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:50
INTERNAL STANDARD	VERIFIED	05:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:50
BLANK TEST	0.00	05:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:51
BLANK TEST	0.00	05:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:53
BLANK TEST	0.00	05:53

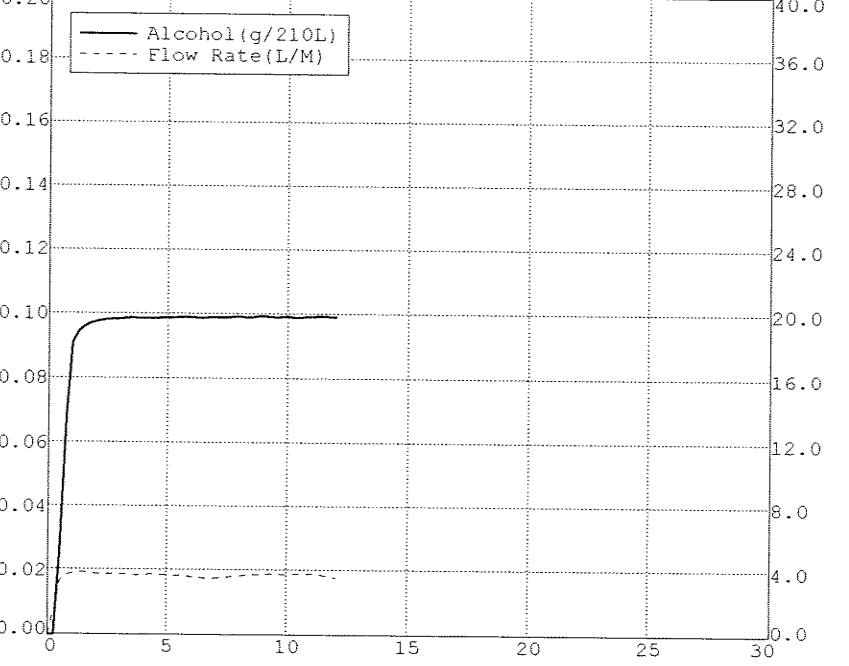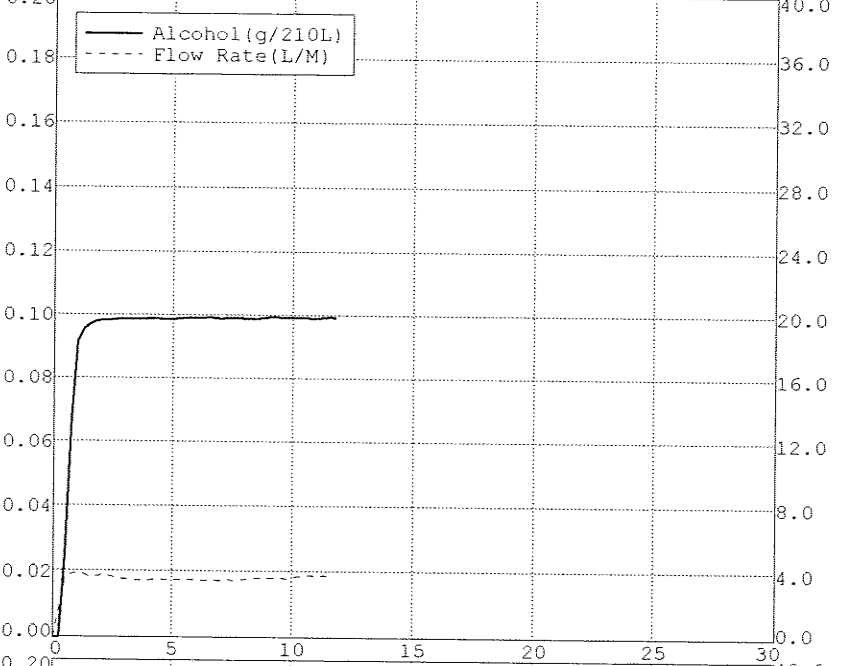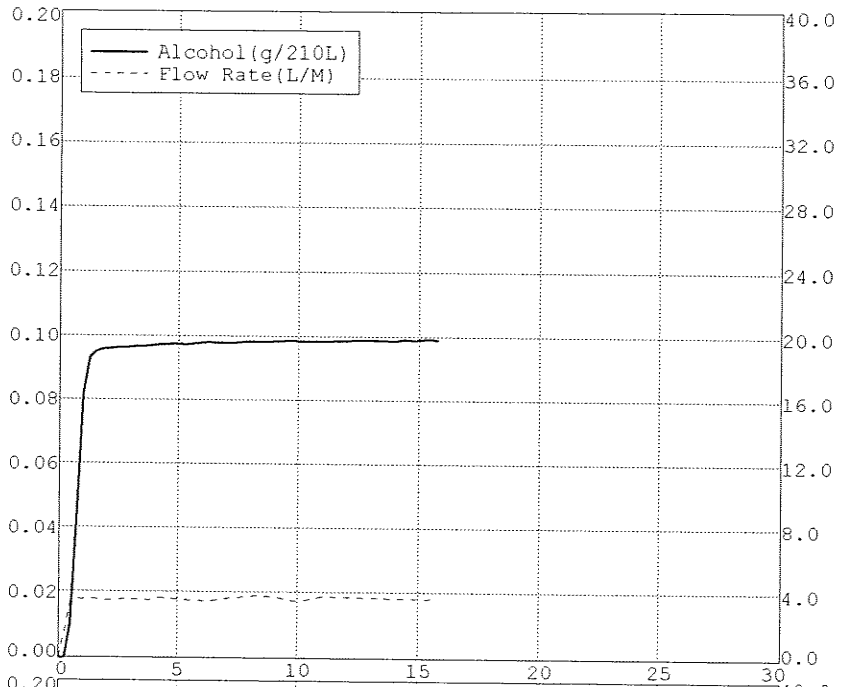

*Handwritten signature and initials*  
#24v