

SUPERVISOR TEST



WARREN COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 02/14/2020

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:57
INTERNAL STANDARD	VERIFIED	13:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:58
BLANK TEST	0.00	13:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:59
BLANK TEST	0.00	14:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:00
BLANK TEST	0.00	14:01

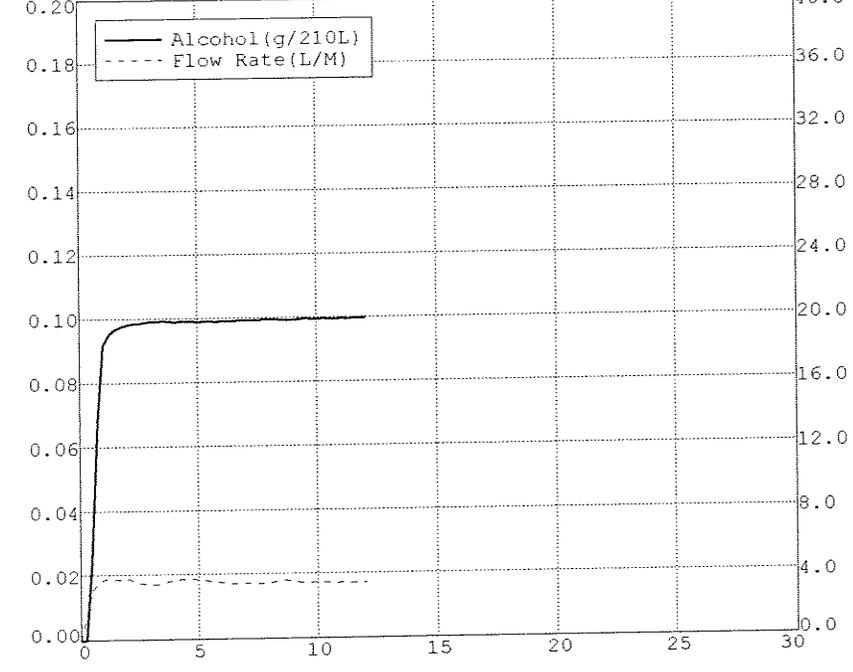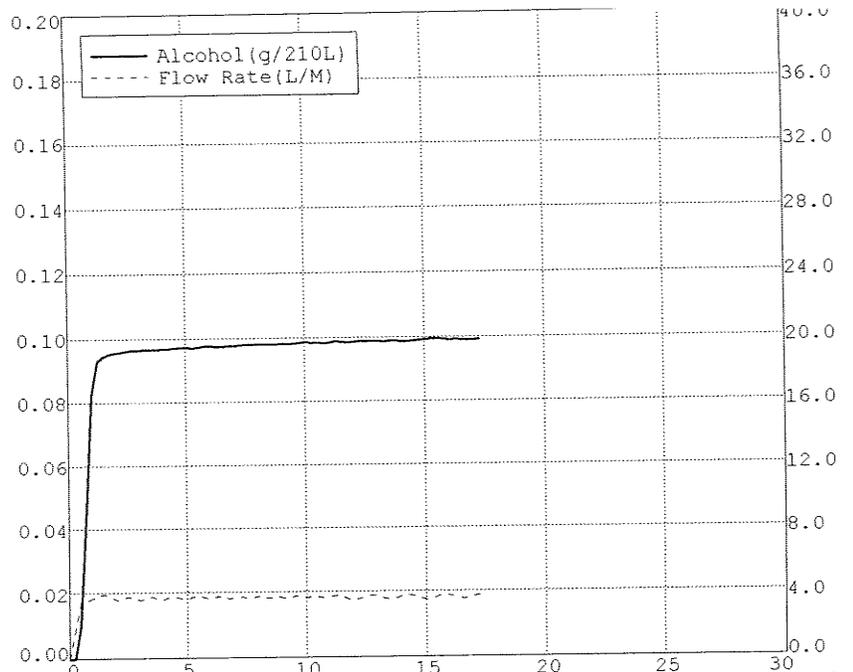

Charles B. Geisler