

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 02/19/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:33
INTERNAL STANDARD	VERIFIED	15:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:33
BLANK TEST	0.00	15:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:35
BLANK TEST	0.00	15:36

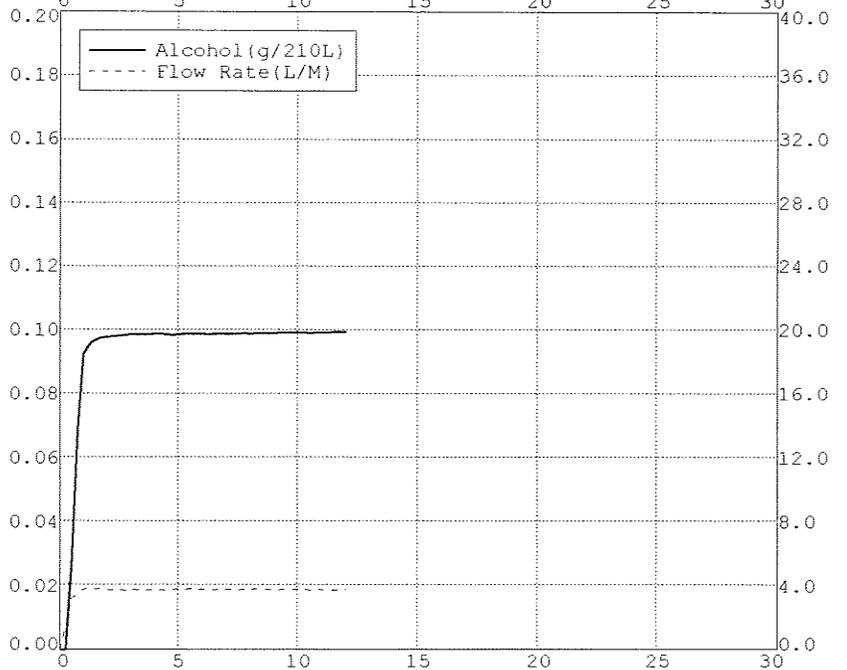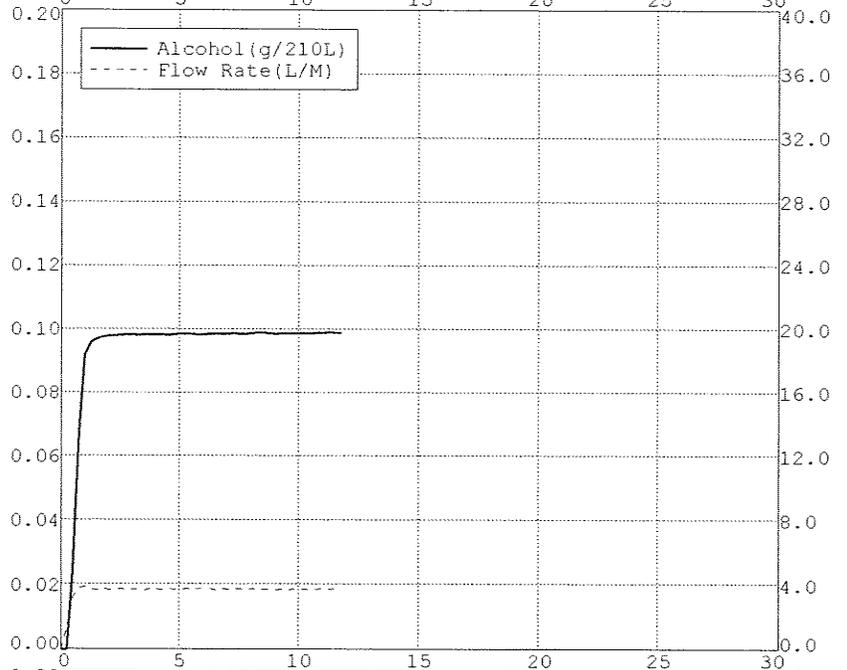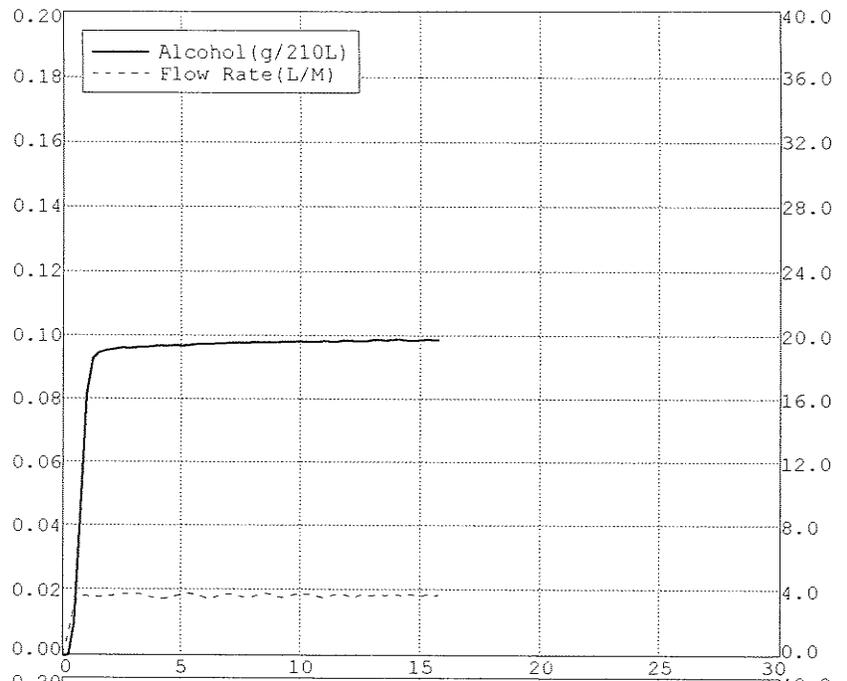

Sgt. C. B. Geisler #2418