

SOLUTION CHANGE




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 03/01/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:54
INTERNAL STANDARD	VERIFIED	13:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:54
BLANK TEST	0.00	13:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:55
BLANK TEST	0.00	13:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:56
BLANK TEST	0.00	13:57

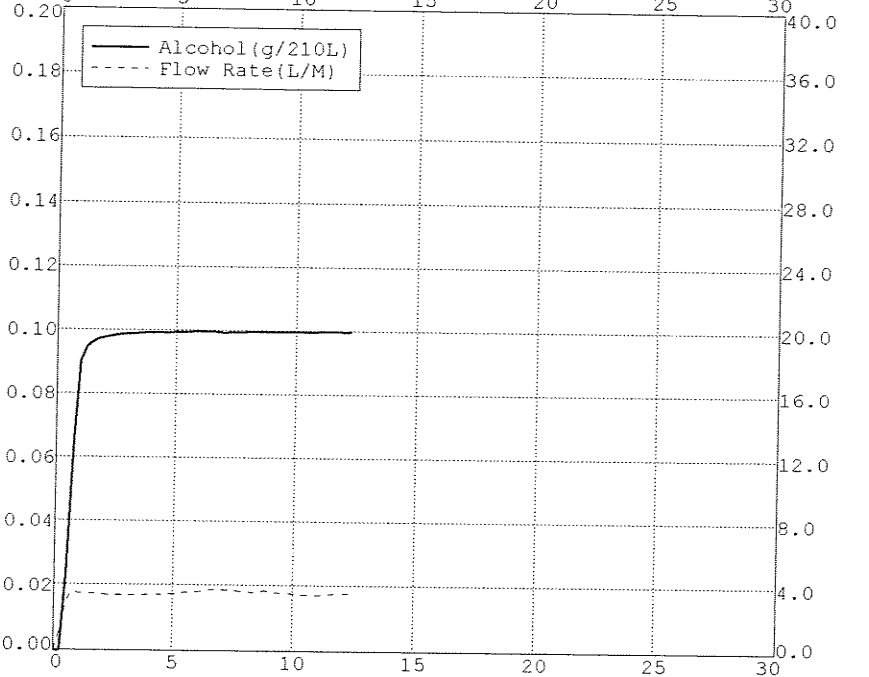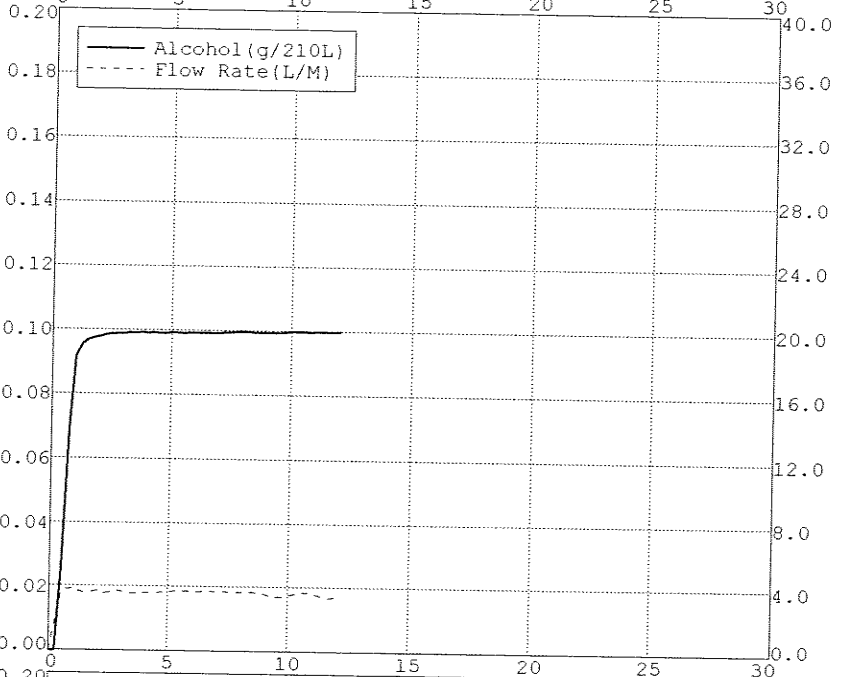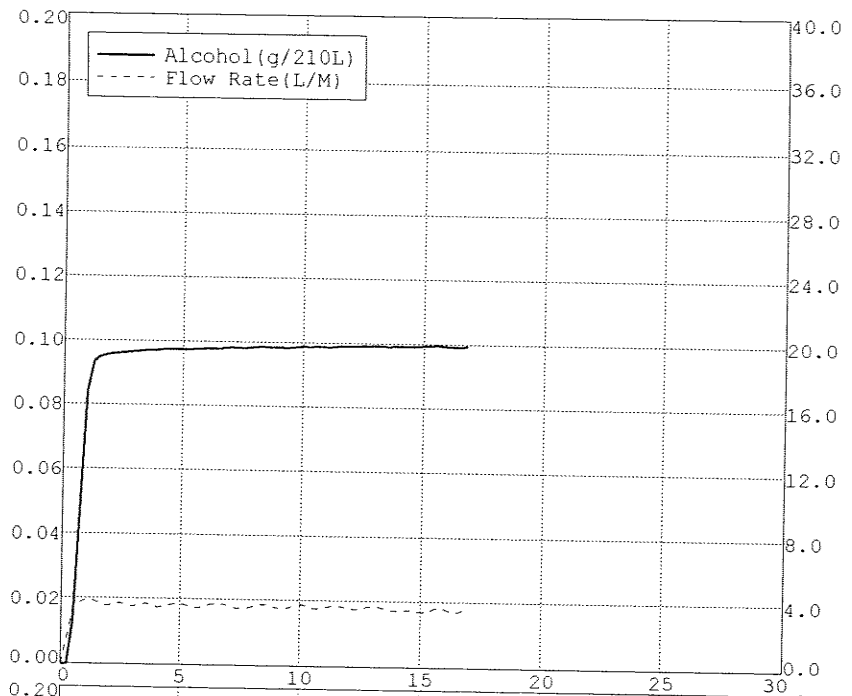

*Charles B. Geisler* # 246