

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 03/09/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:39
INTERNAL STANDARD	VERIFIED	16:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:39
BLANK TEST	0.00	16:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:41
BLANK TEST	0.00	16:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:42
BLANK TEST	0.00	16:43

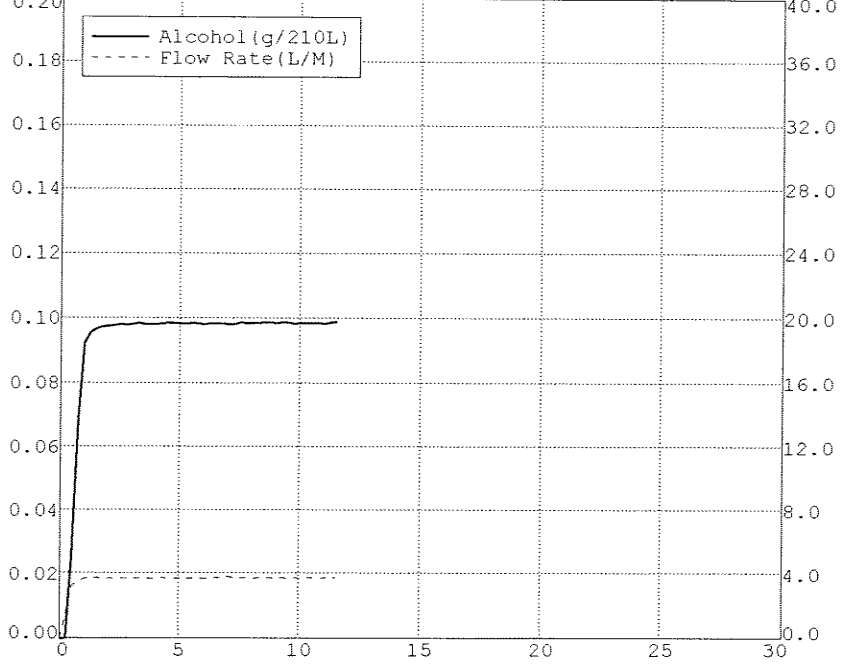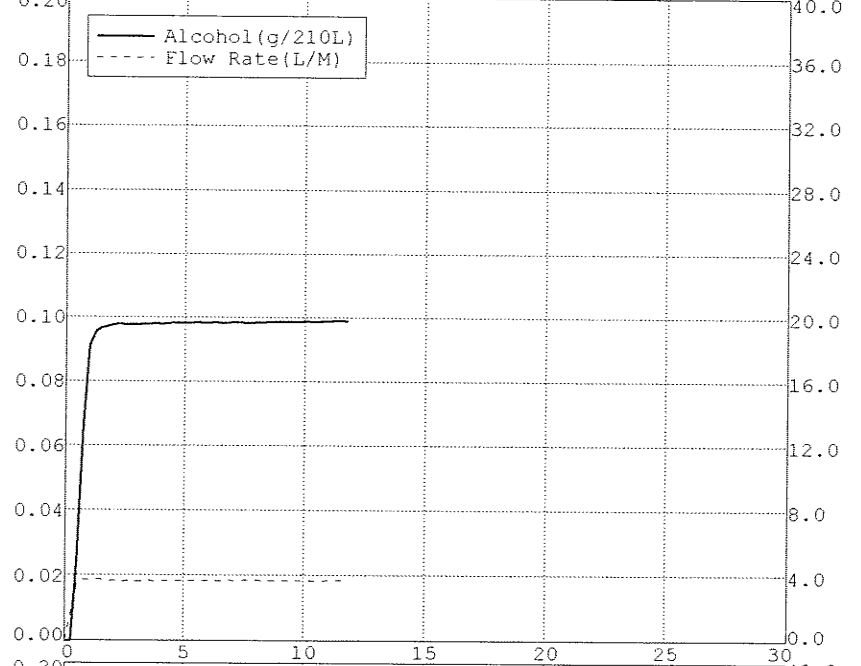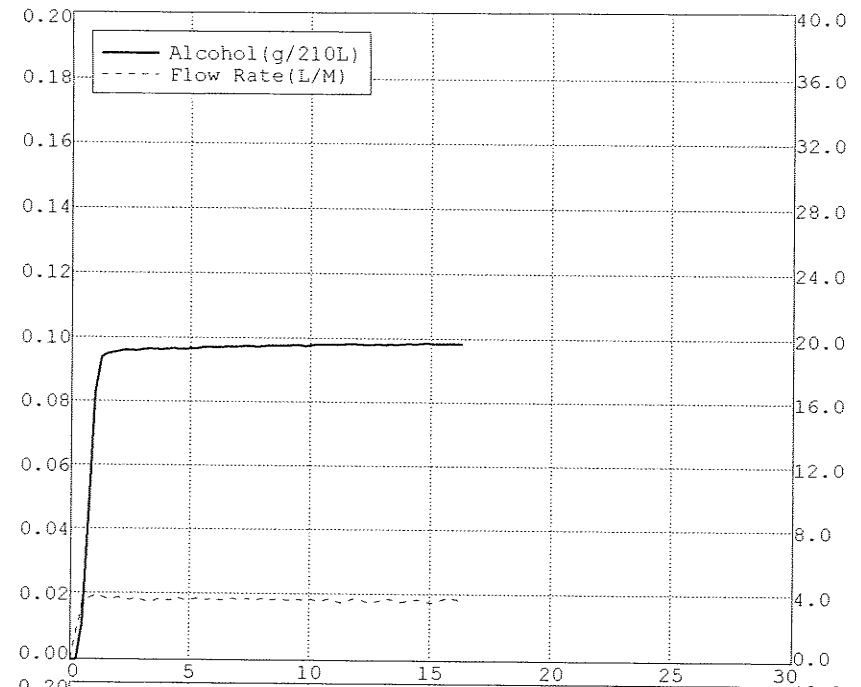

Signature: Sgt. Charles B. Geisler #248