

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 04/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:16
INTERNAL STANDARD	VERIFIED	17:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:17
BLANK TEST	0.00	17:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:18
BLANK TEST	0.00	17:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:19
BLANK TEST	0.00	17:20

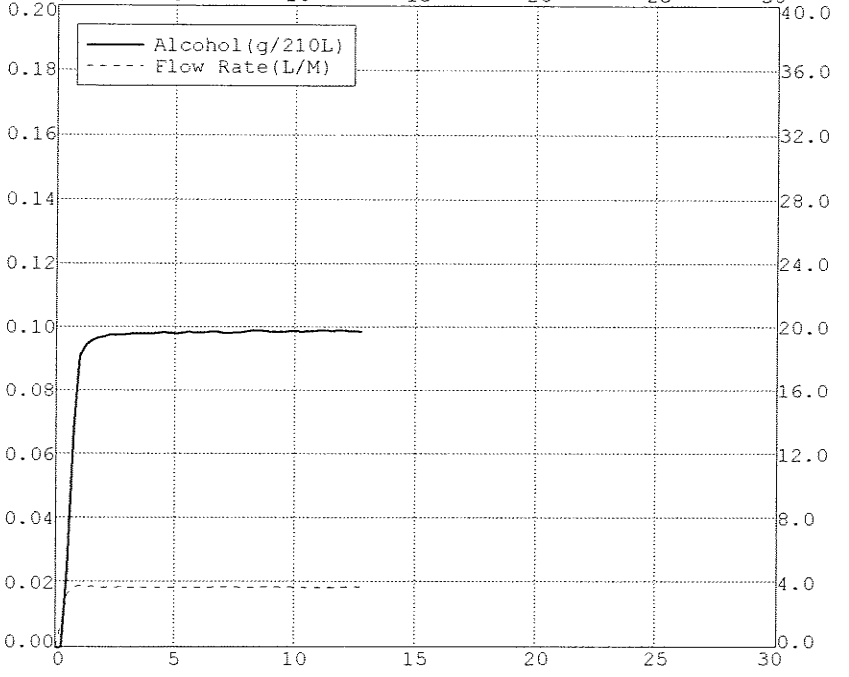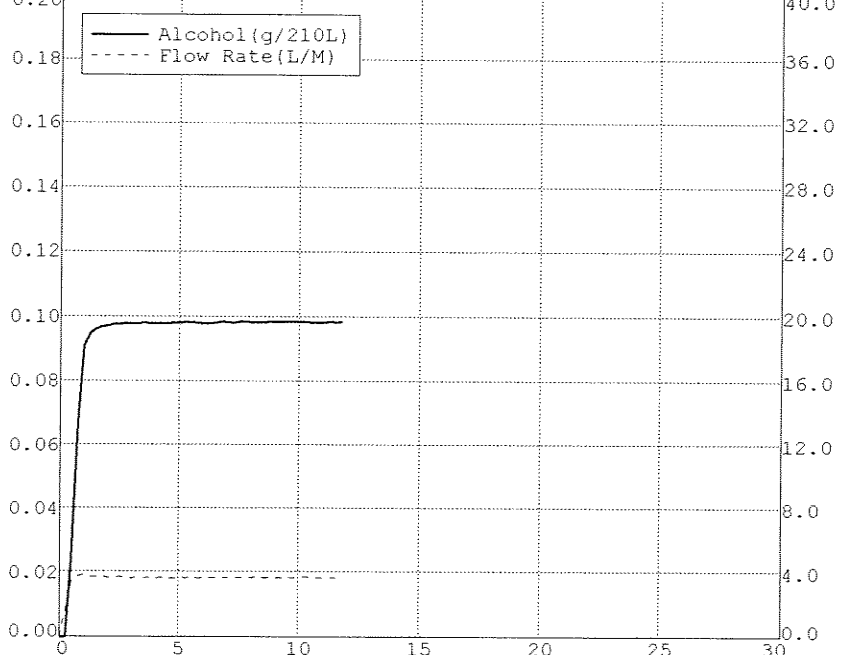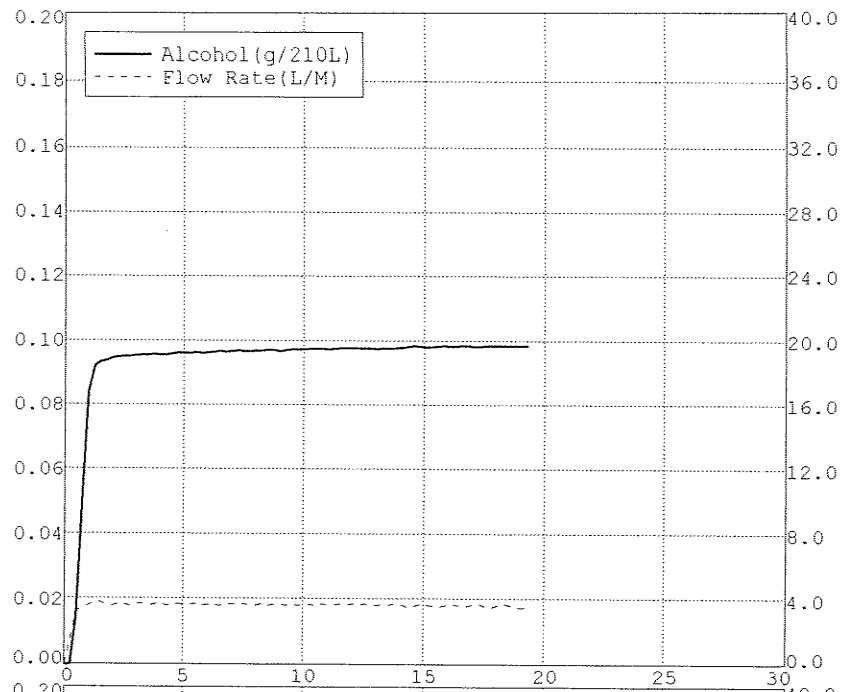

Handwritten signature and initials
2041