

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 04/07/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:51
INTERNAL STANDARD	VERIFIED	13:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:51
BLANK TEST	0.00	13:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:53
BLANK TEST	0.00	13:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:54
BLANK TEST	0.00	13:55

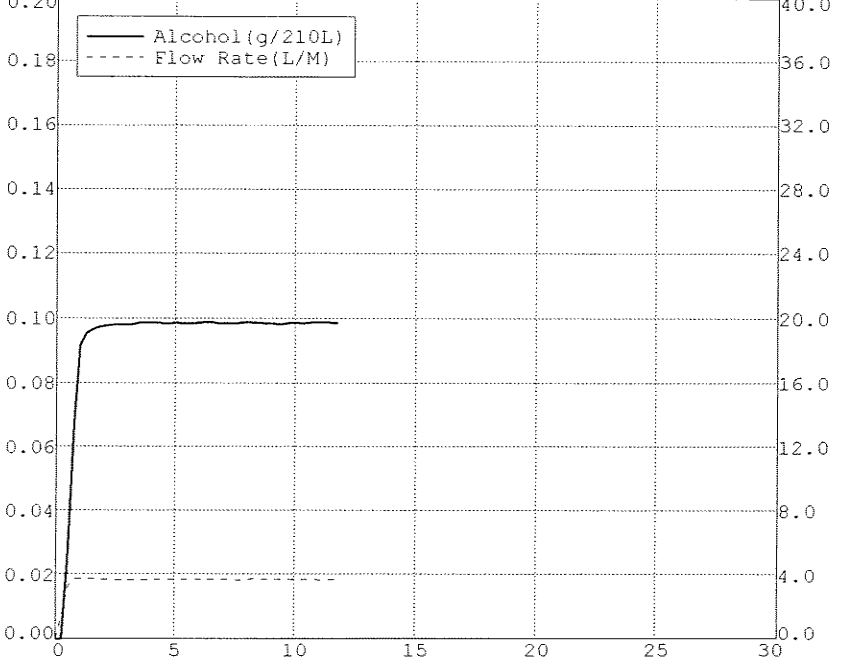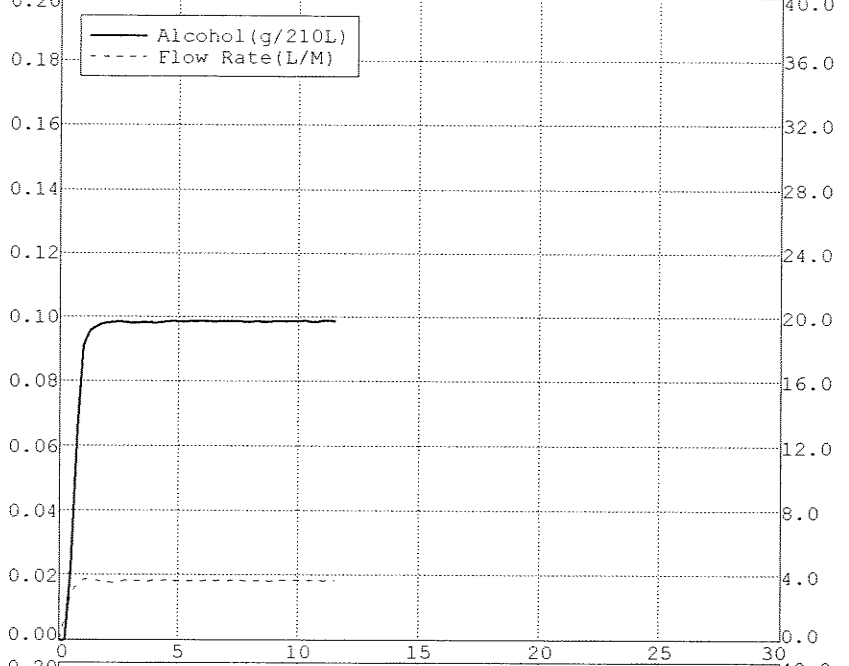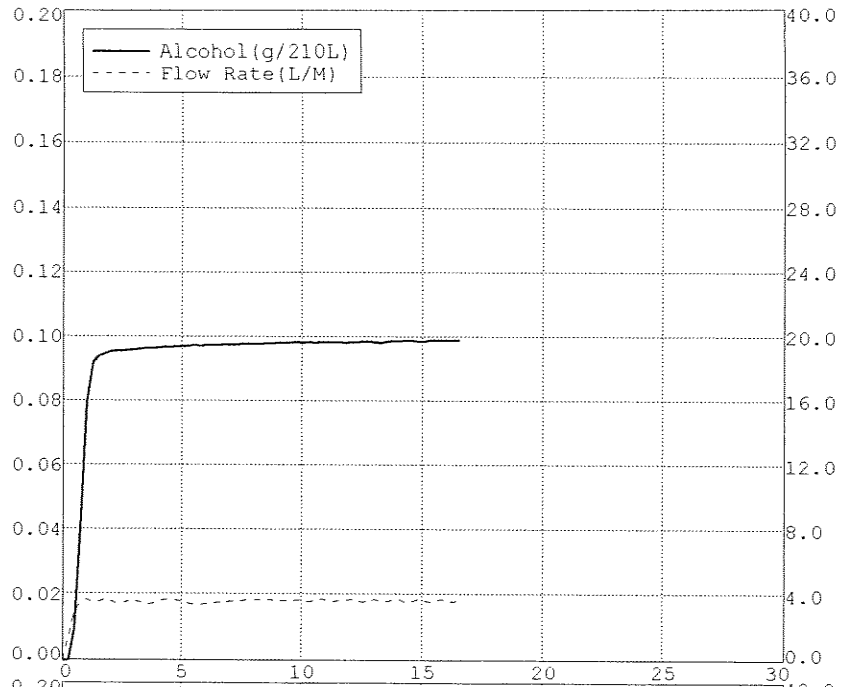

*Signature: Sgt. C. B. Geisler*