

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 04/15/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:44
INTERNAL STANDARD	VERIFIED	12:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:45
BLANK TEST	0.00	12:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:47
BLANK TEST	0.00	12:47

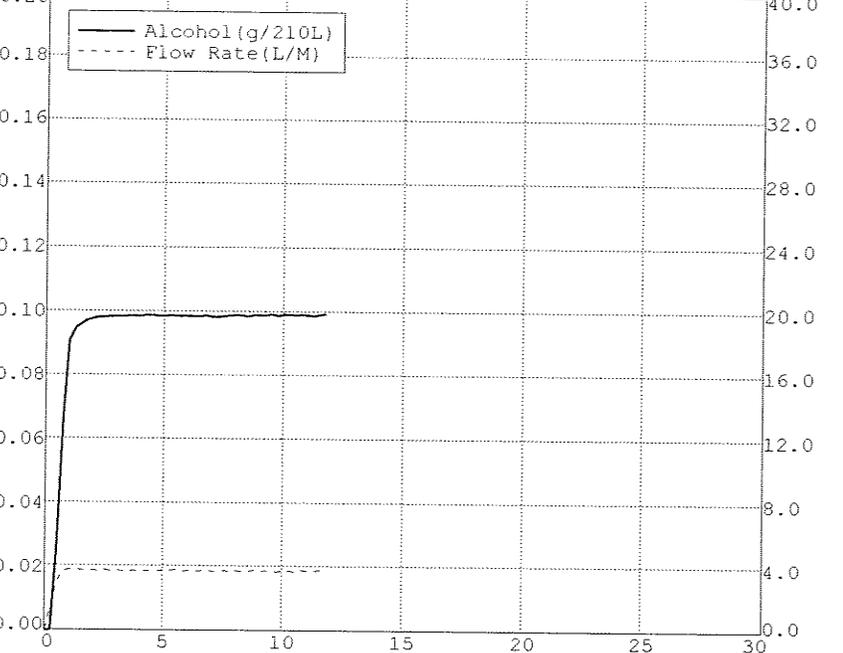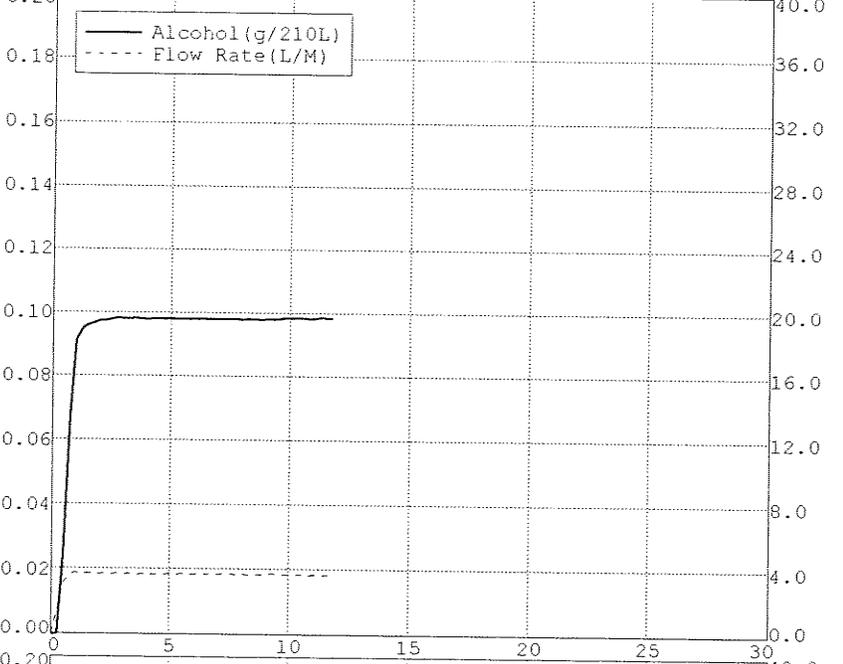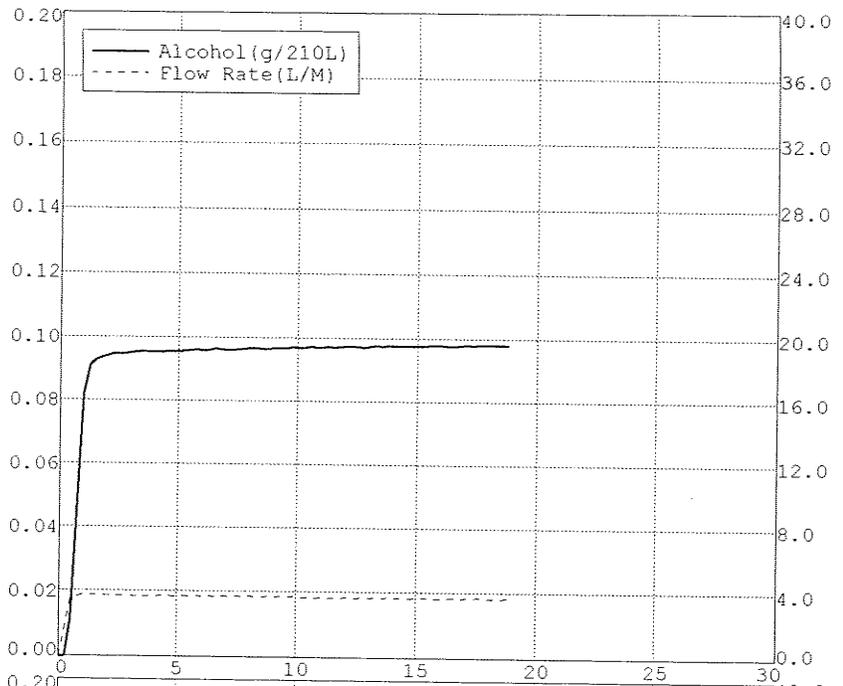

*dgf. Chl - B. #24 ✓*