

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 04/21/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:19
INTERNAL STANDARD	VERIFIED	14:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:20
BLANK TEST	0.00	14:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:21
BLANK TEST	0.00	14:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:22
BLANK TEST	0.00	14:23

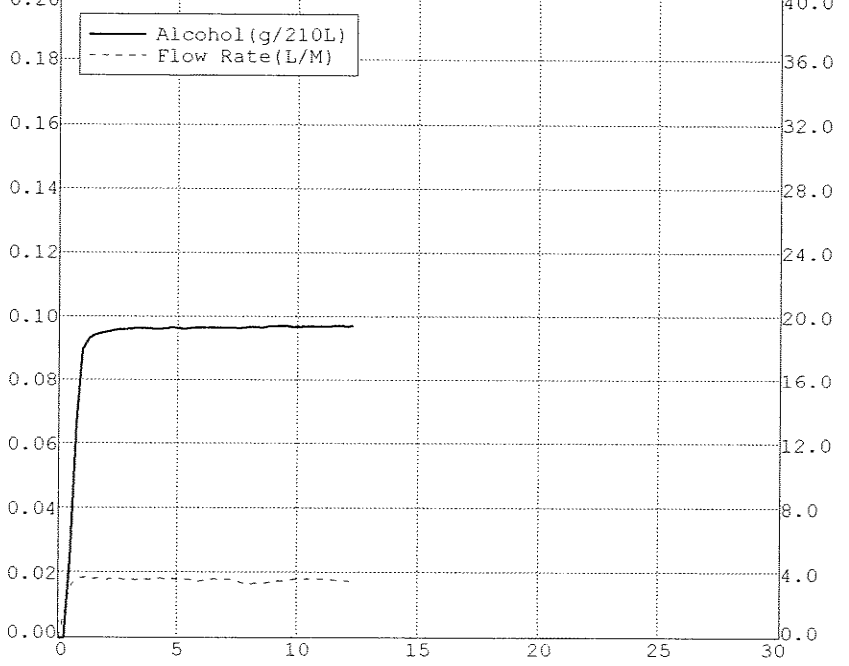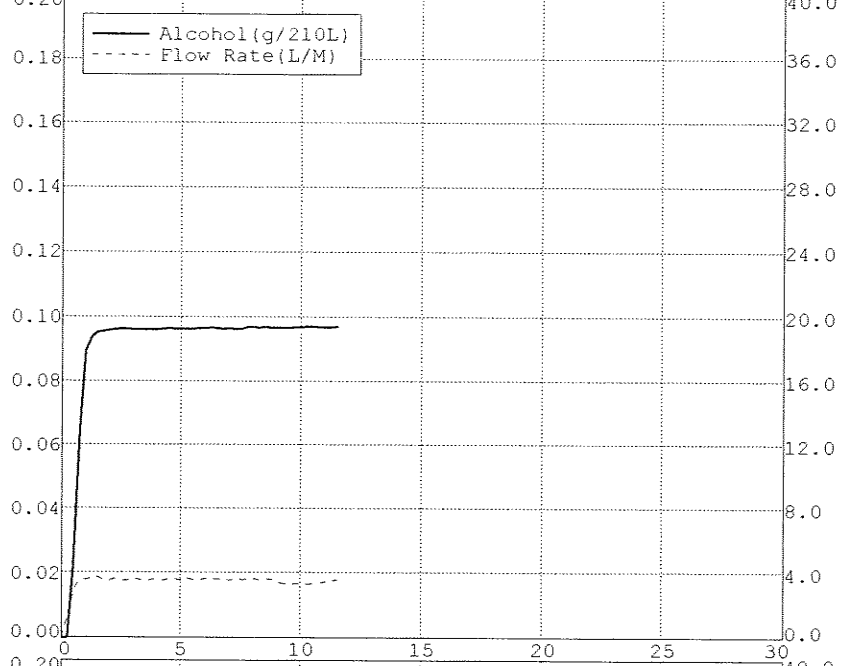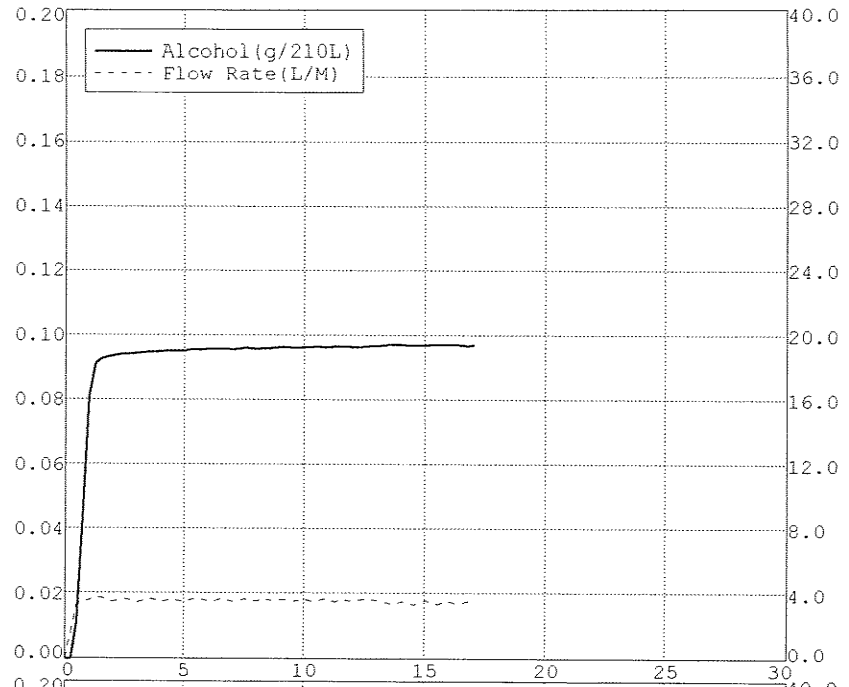

Charles B. Geisler
#2115