

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/13/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:00
INTERNAL STANDARD	VERIFIED	14:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:00
BLANK TEST	0.00	14:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:02
BLANK TEST	0.00	14:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:03
BLANK TEST	0.00	14:04

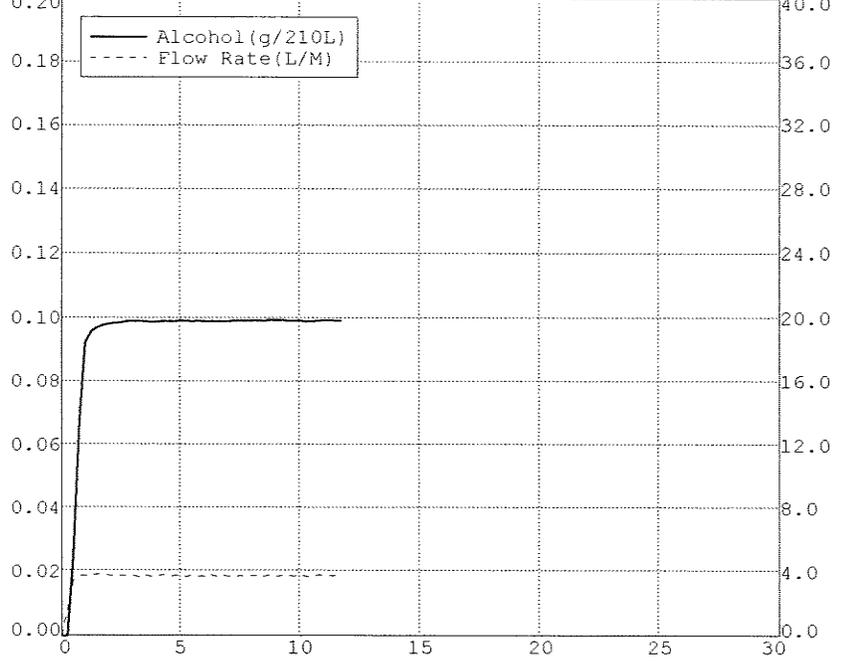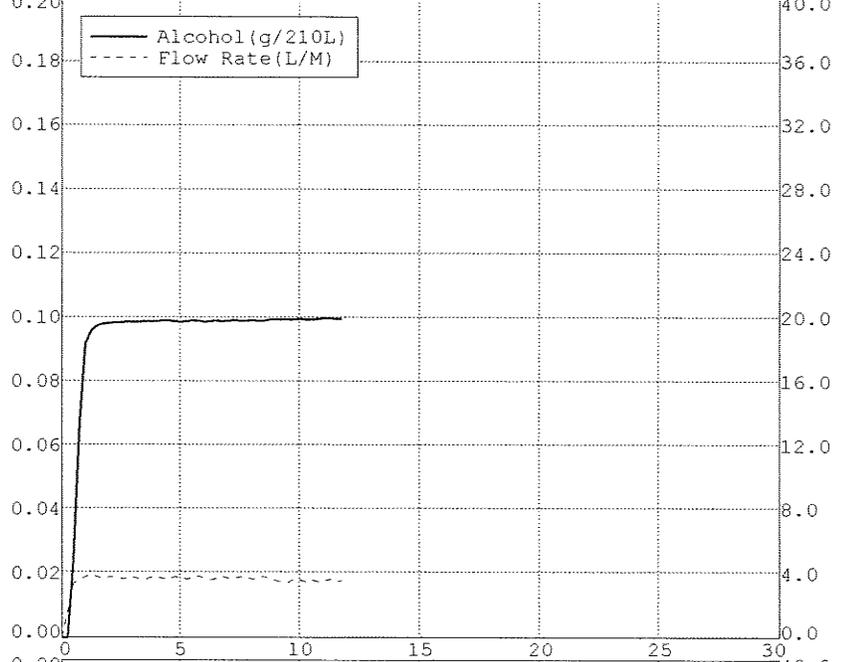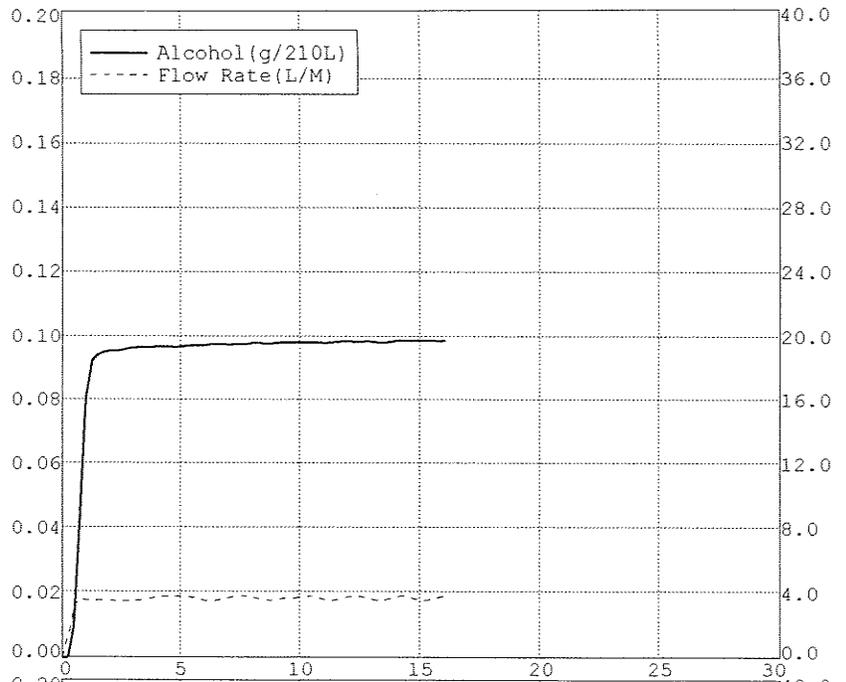

Charles B. Geisler