

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/19/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:36
INTERNAL STANDARD	VERIFIED	16:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:37
BLANK TEST	0.00	16:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:38
BLANK TEST	0.00	16:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:39
BLANK TEST	0.00	16:40

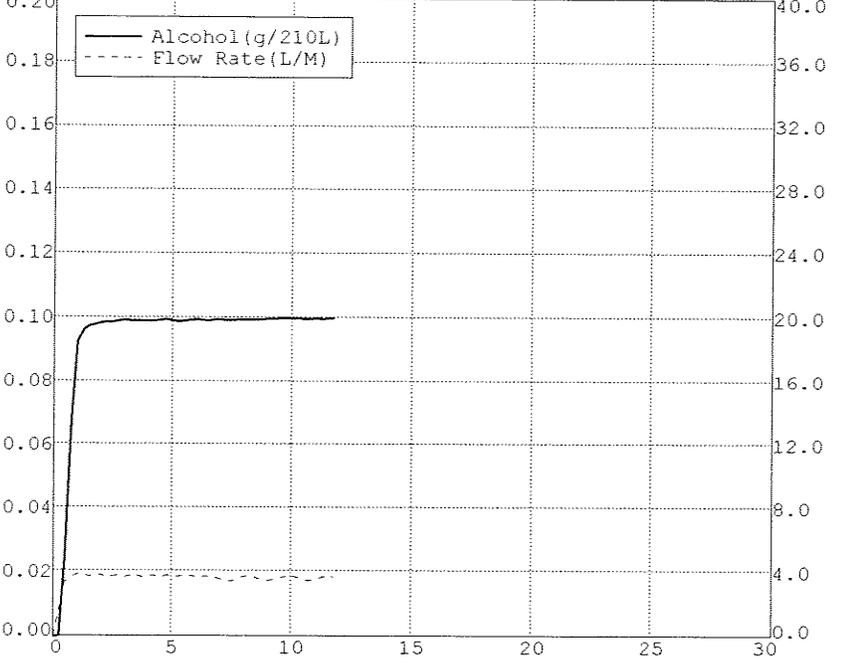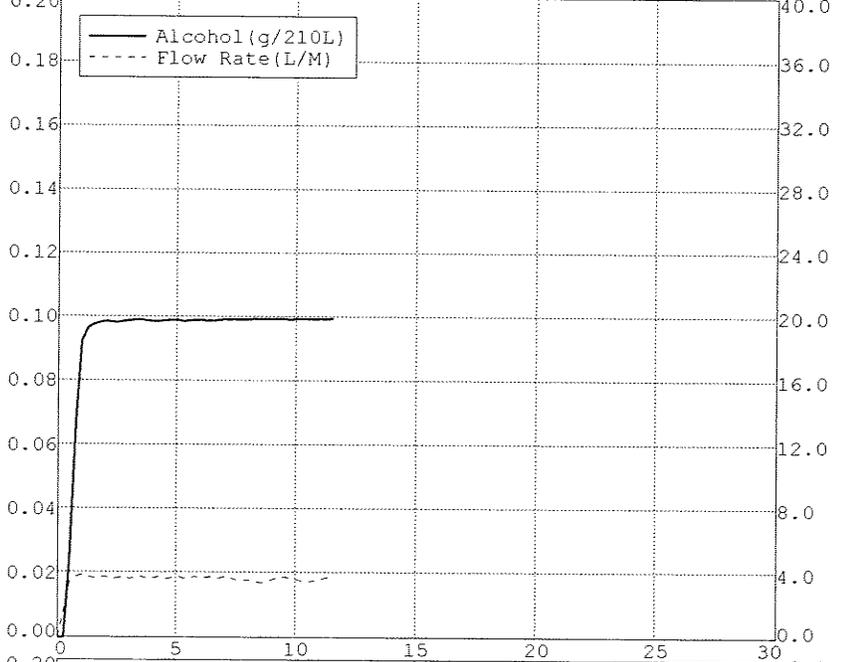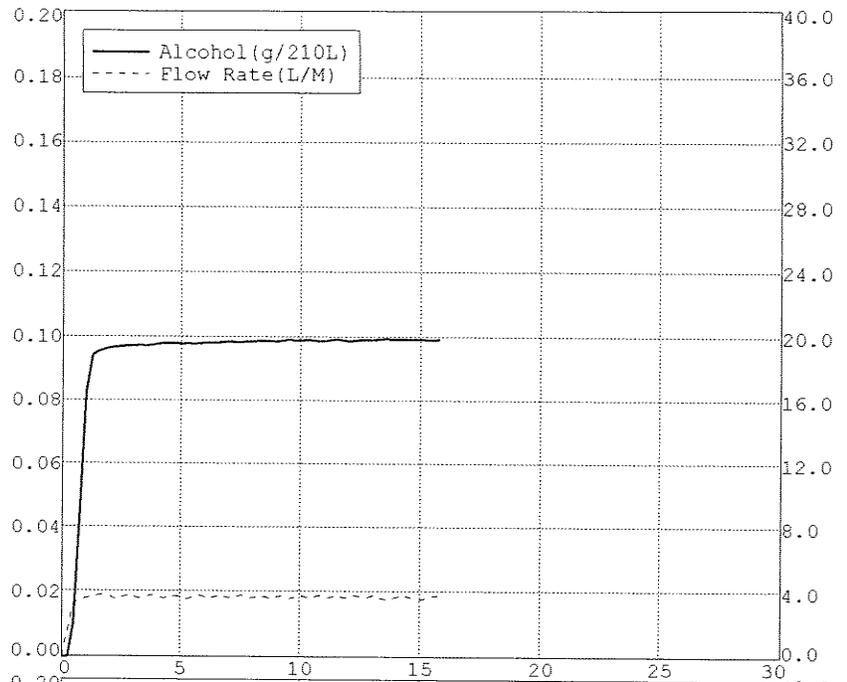

Sgt. C. B. Geisler
5/19/2020