

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 06/15/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:11
INTERNAL STANDARD	VERIFIED	15:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:12
BLANK TEST	0.00	15:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:13
BLANK TEST	0.00	15:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:14
BLANK TEST	0.00	15:15

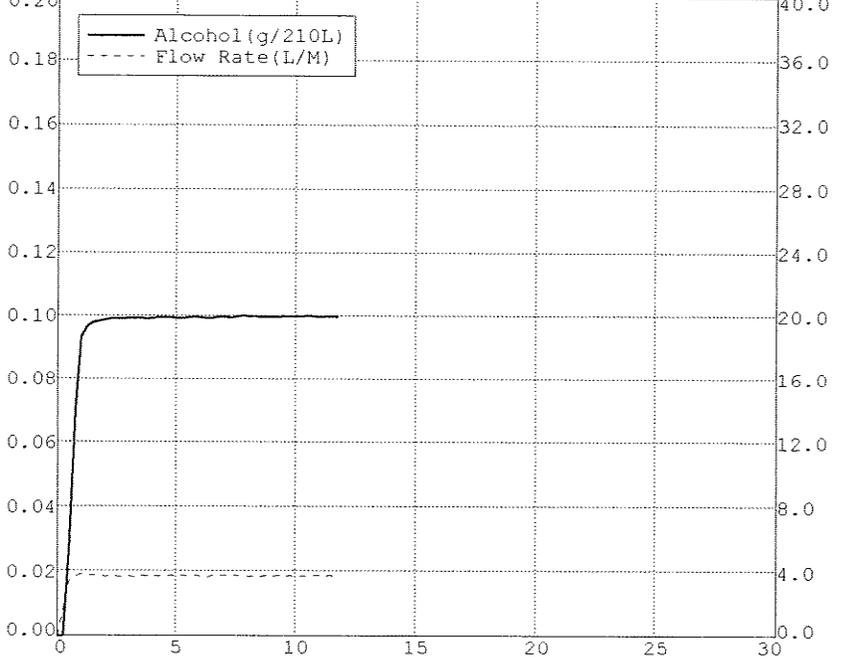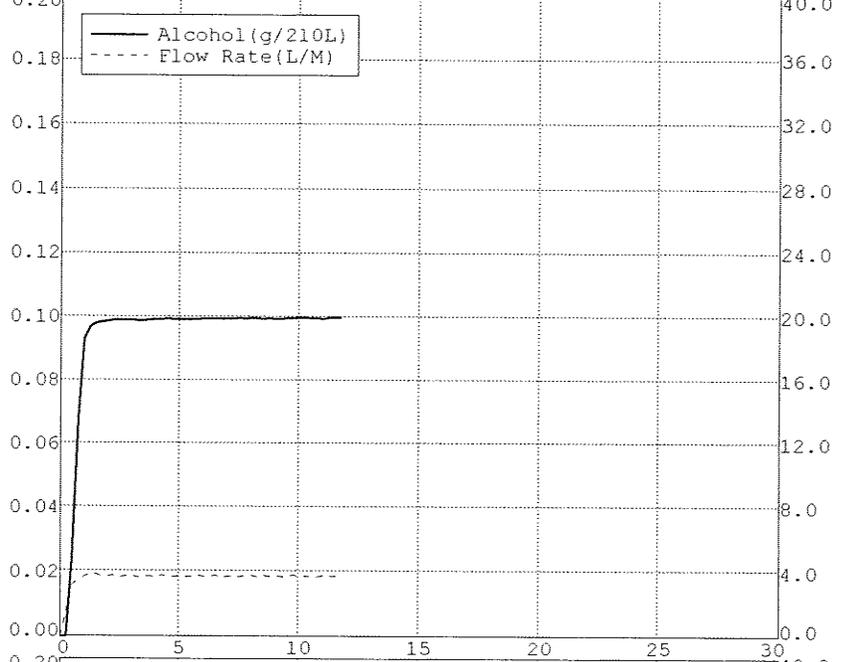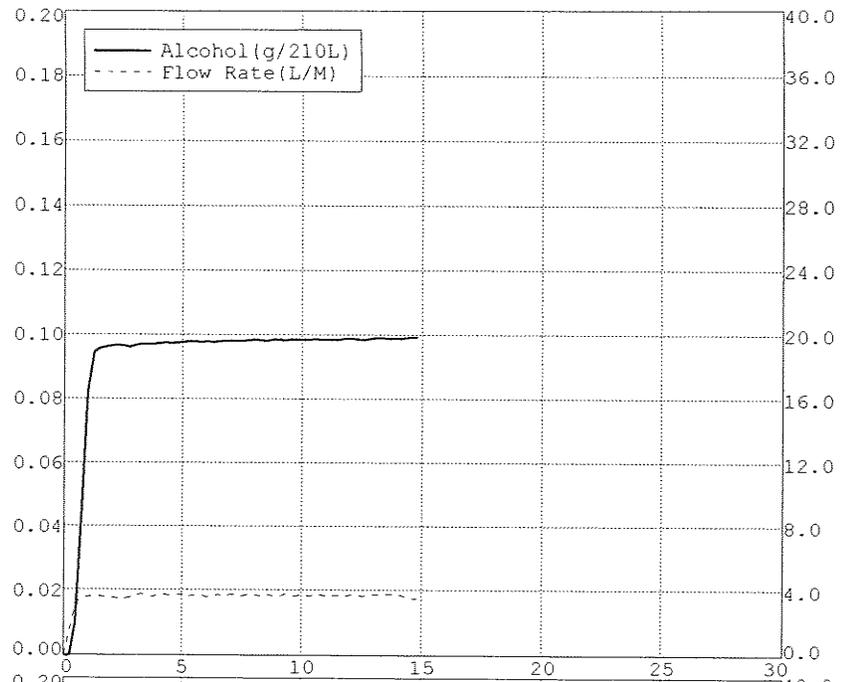

Charles B. Geisler