

SUPERVISOR TEST




WARREN COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 06/21/2020

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:56
INTERNAL STANDARD	VERIFIED	16:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:57
BLANK TEST	0.00	16:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:58
BLANK TEST	0.00	16:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:59
BLANK TEST	0.00	17:00

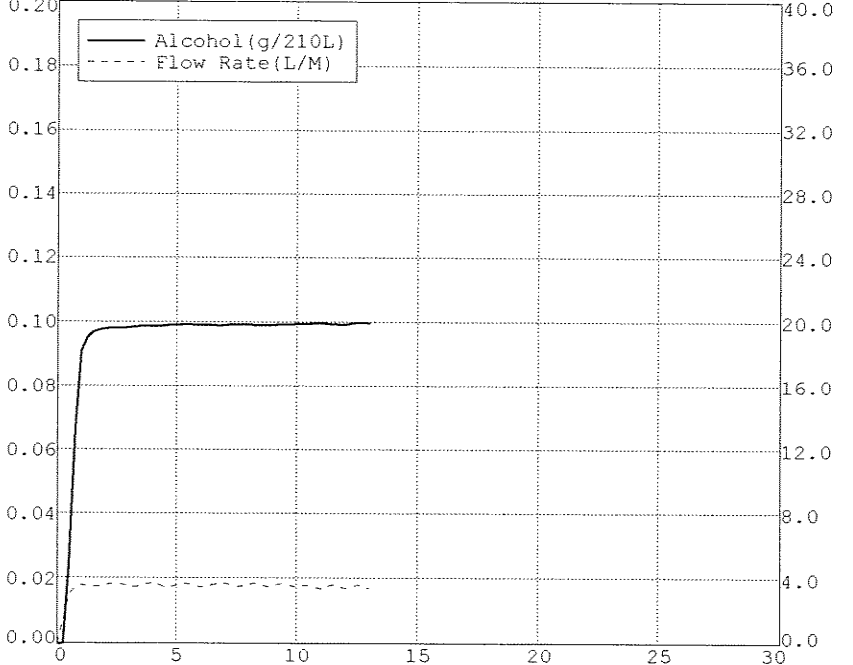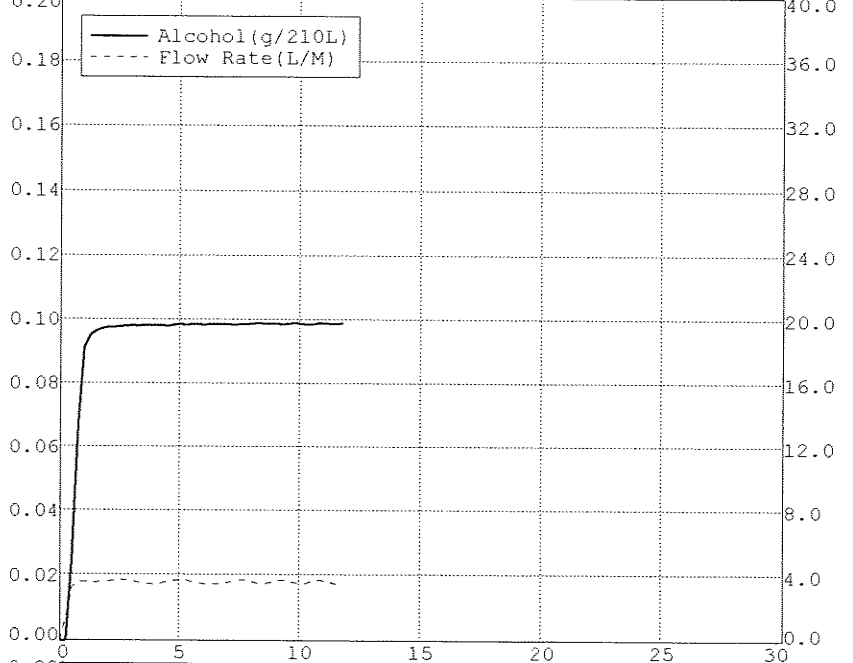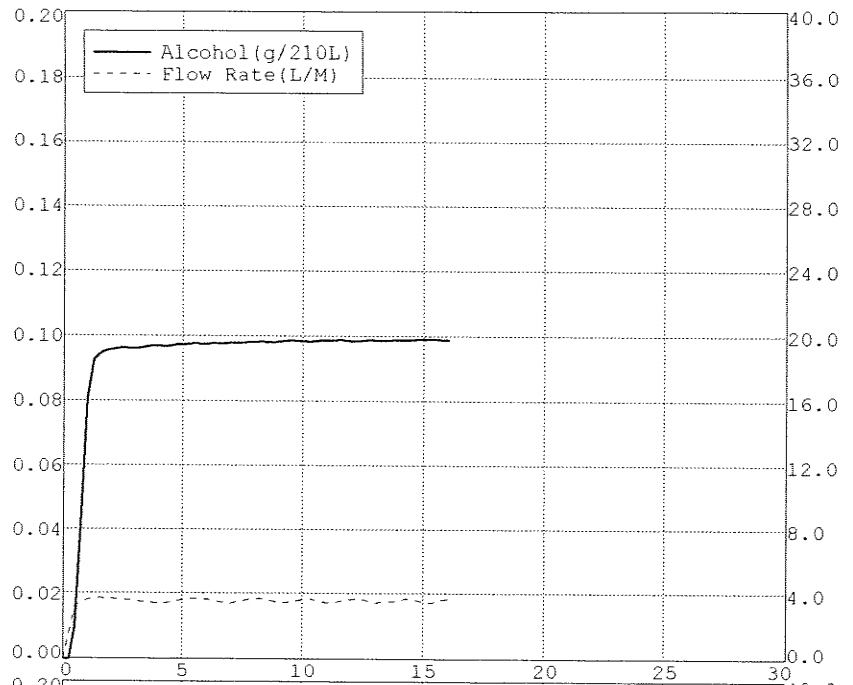

Signature: Sgt. Charles B. Geisler #241