

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/03/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:29
INTERNAL STANDARD	VERIFIED	16:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:30
BLANK TEST	0.00	16:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:31
BLANK TEST	0.00	16:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:32
BLANK TEST	0.00	16:33

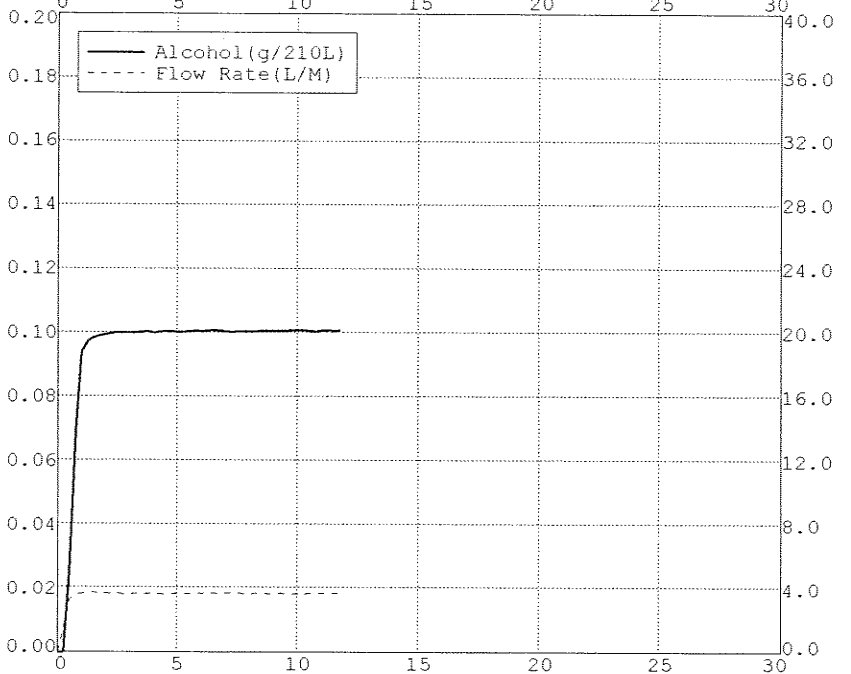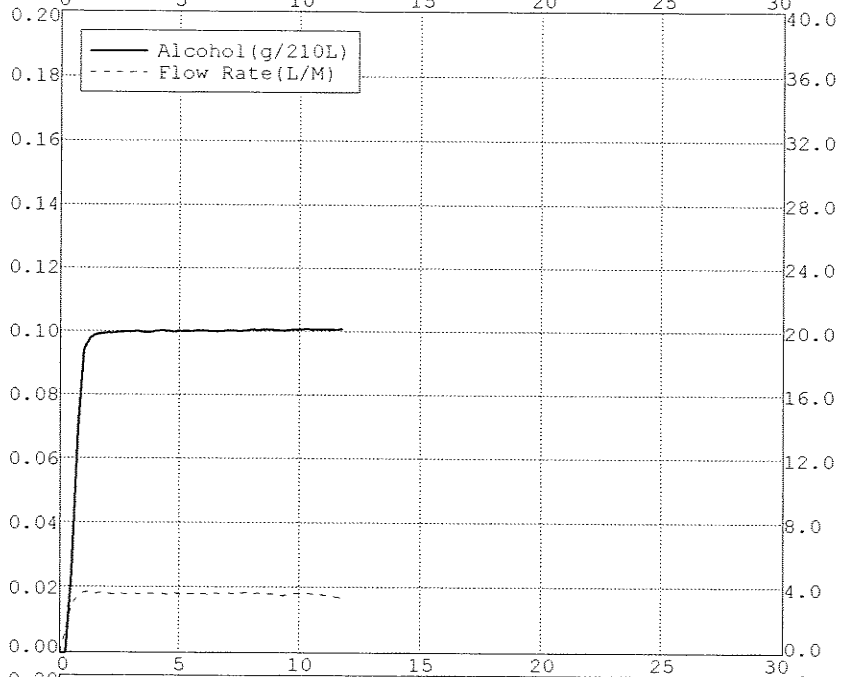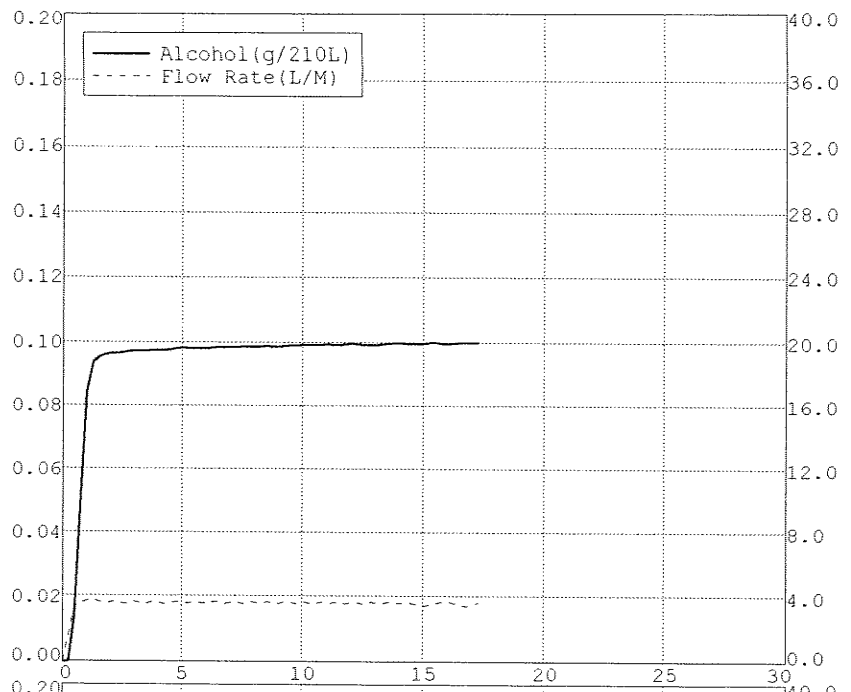

Sp. Ch. B. [Signature] #241