

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/22/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:21
INTERNAL STANDARD	VERIFIED	17:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:22
BLANK TEST	0.00	17:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:23
BLANK TEST	0.00	17:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:24
BLANK TEST	0.00	17:25

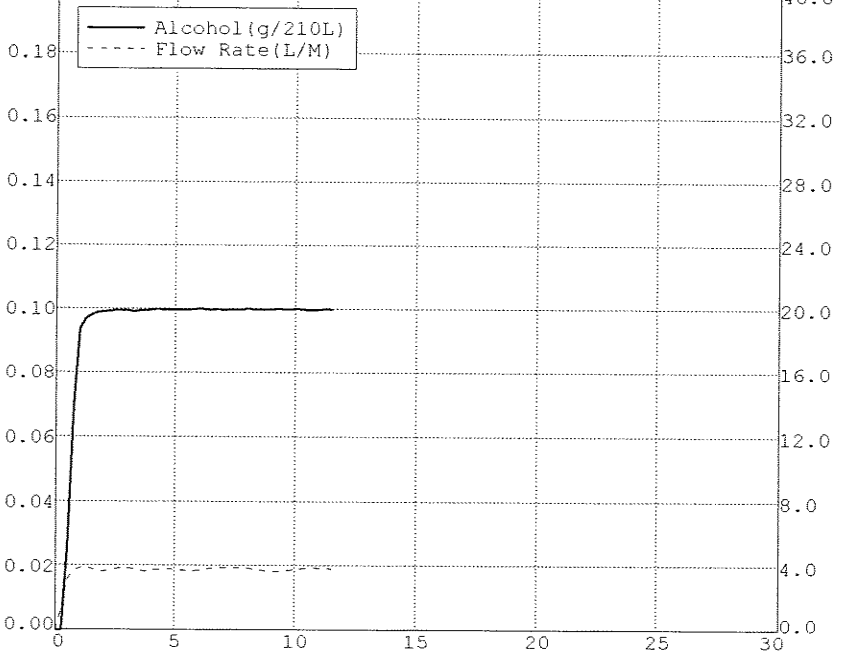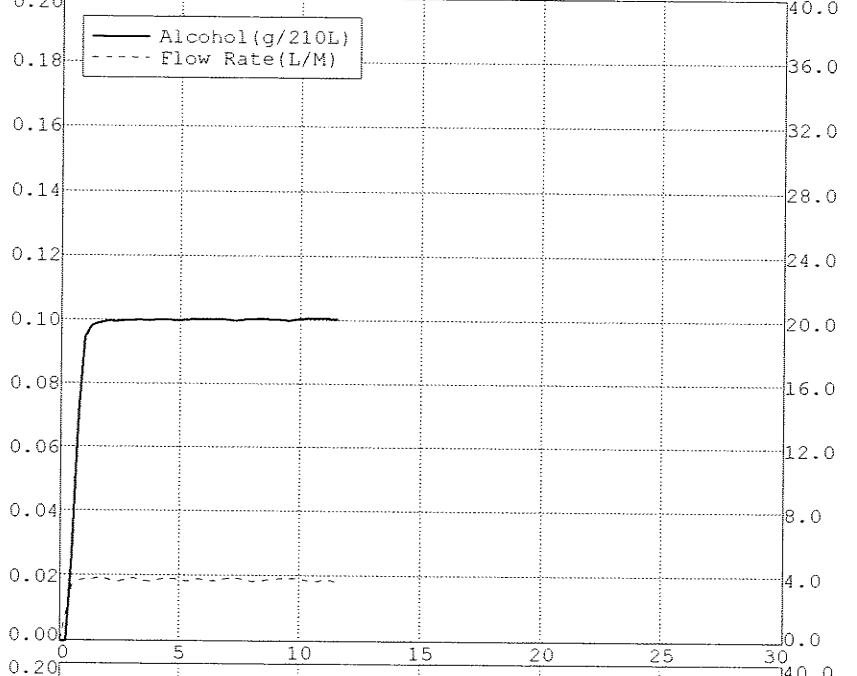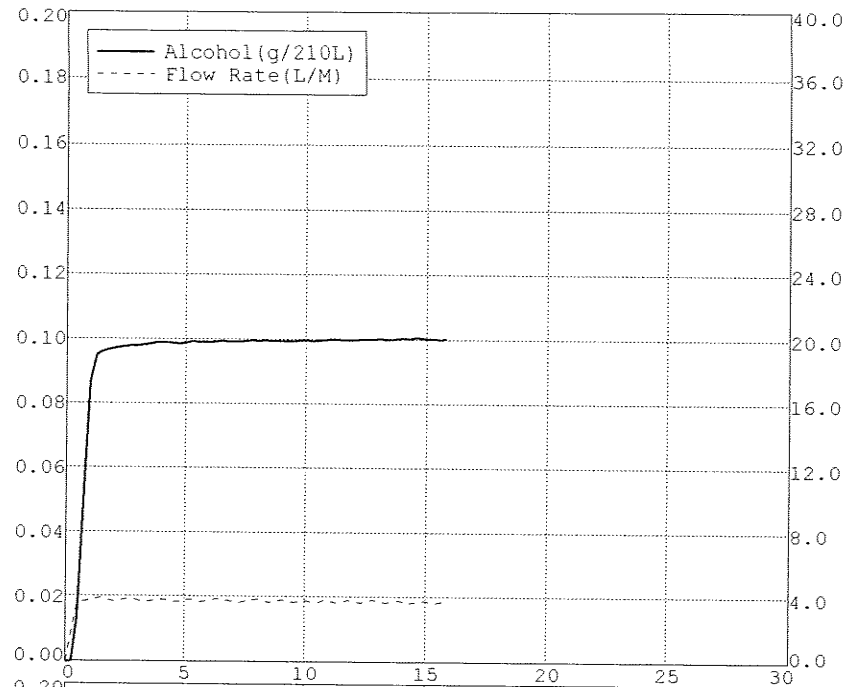

Signature: C. B. Geisler
#224