

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/14/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:53
INTERNAL STANDARD	VERIFIED	13:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:53
BLANK TEST	0.00	13:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:54
BLANK TEST	0.00	13:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:56
BLANK TEST	0.00	13:56

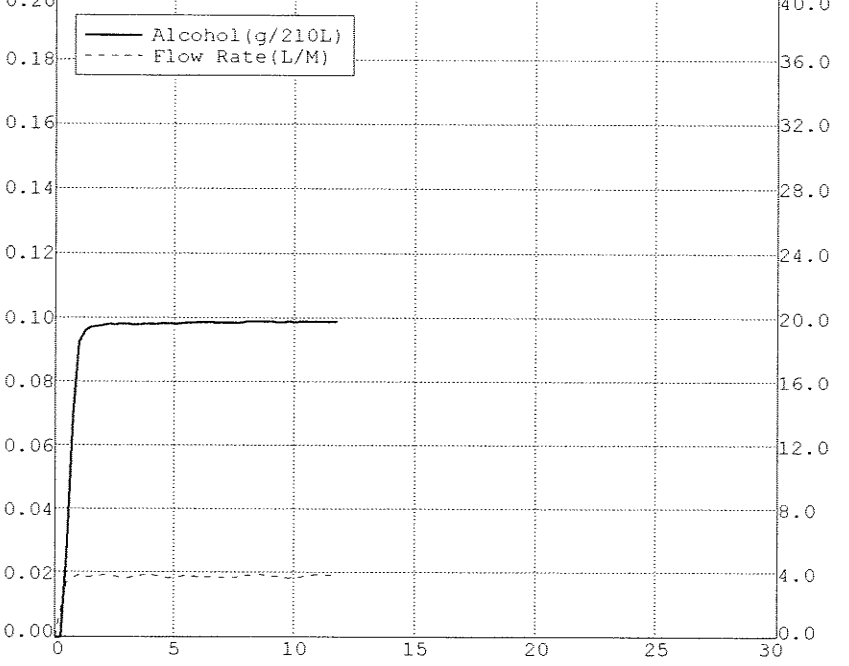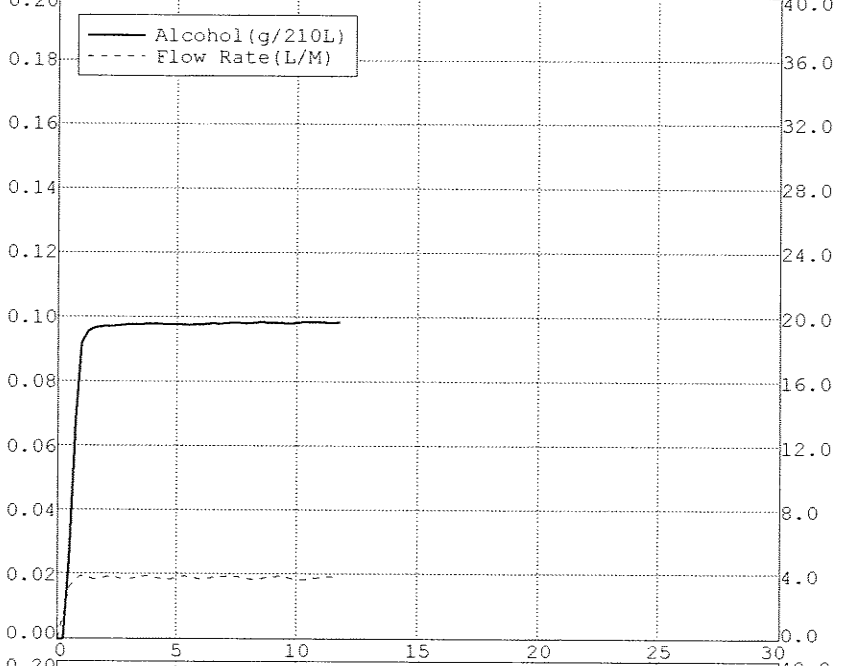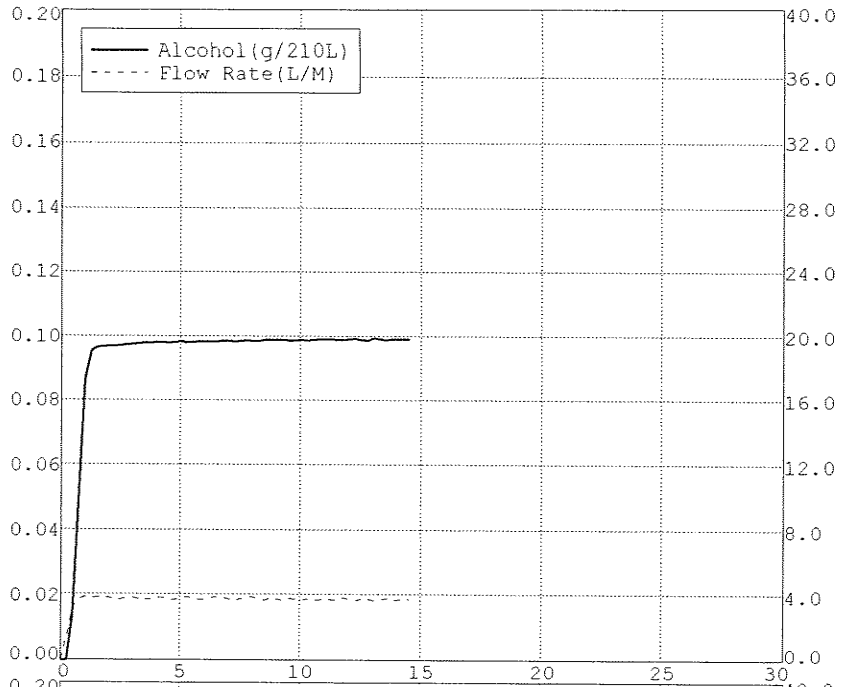

Handwritten signature: C. B. Geisler #20240