

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 09/08/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:24
INTERNAL STANDARD	VERIFIED	16:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:25
BLANK TEST	0.00	16:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:26
BLANK TEST	0.00	16:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:27
BLANK TEST	0.00	16:28

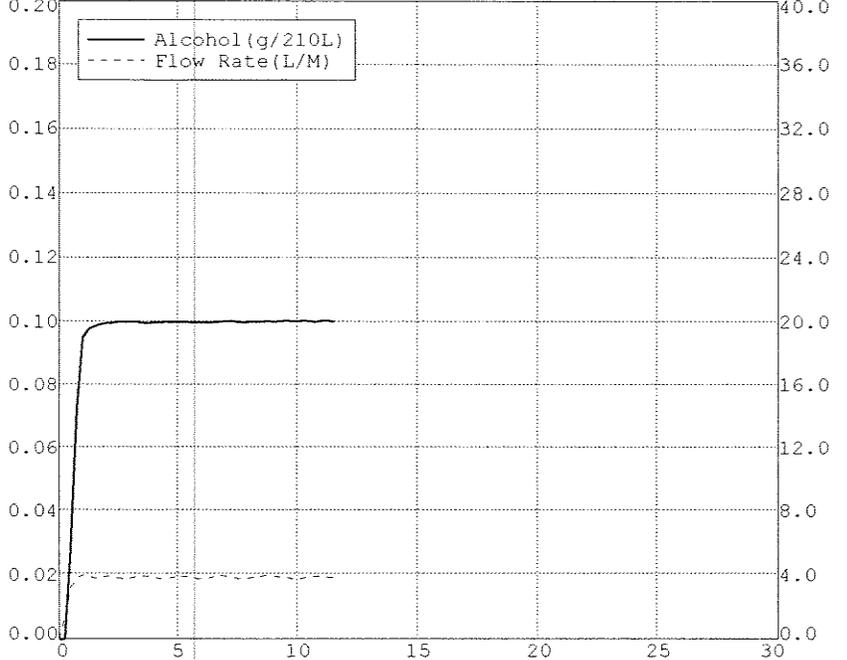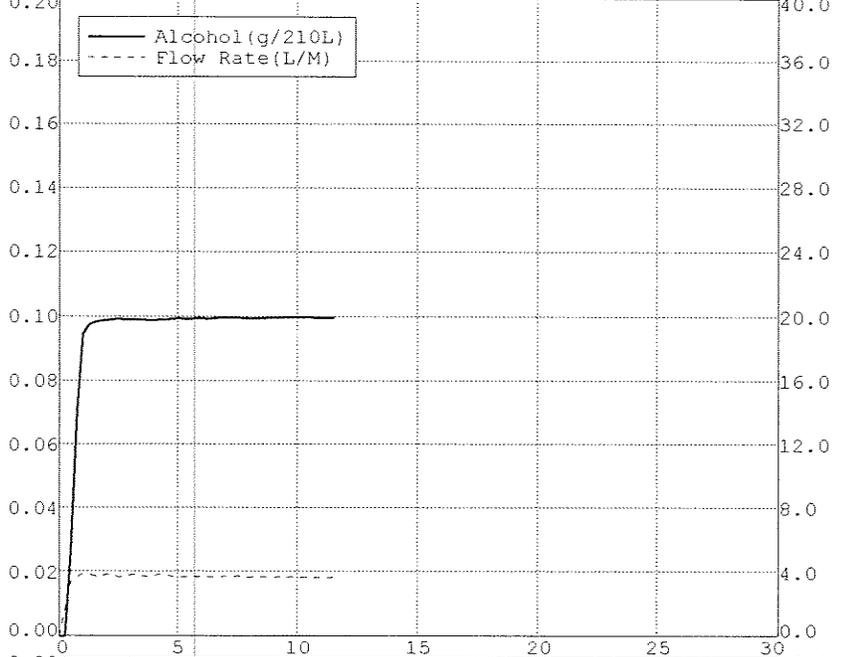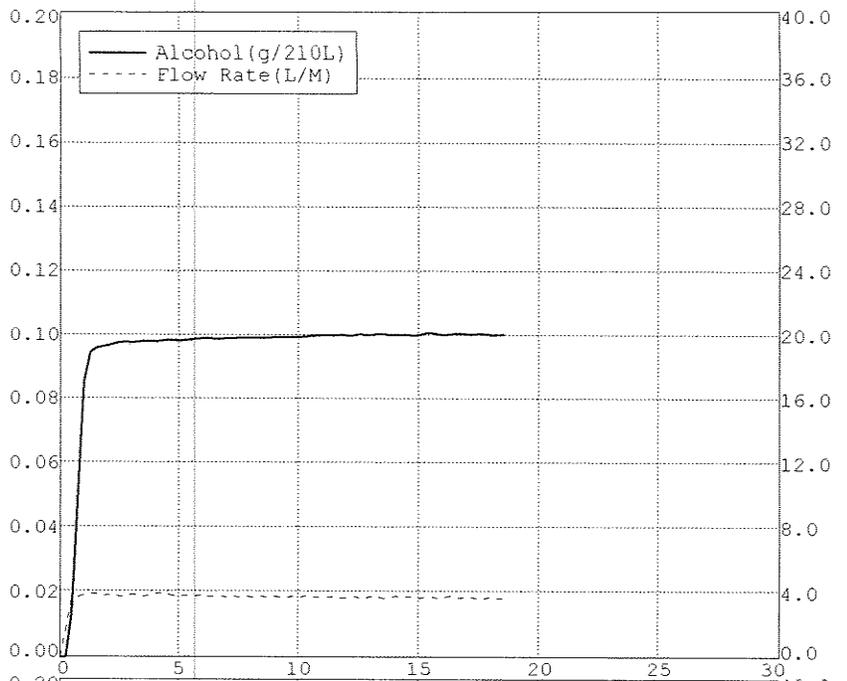

Sgt. Charles B. Geisler #245