

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 10/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:21
INTERNAL STANDARD	VERIFIED	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:21
BLANK TEST	0.00	16:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:22
BLANK TEST	0.00	16:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:24
BLANK TEST	0.00	16:25

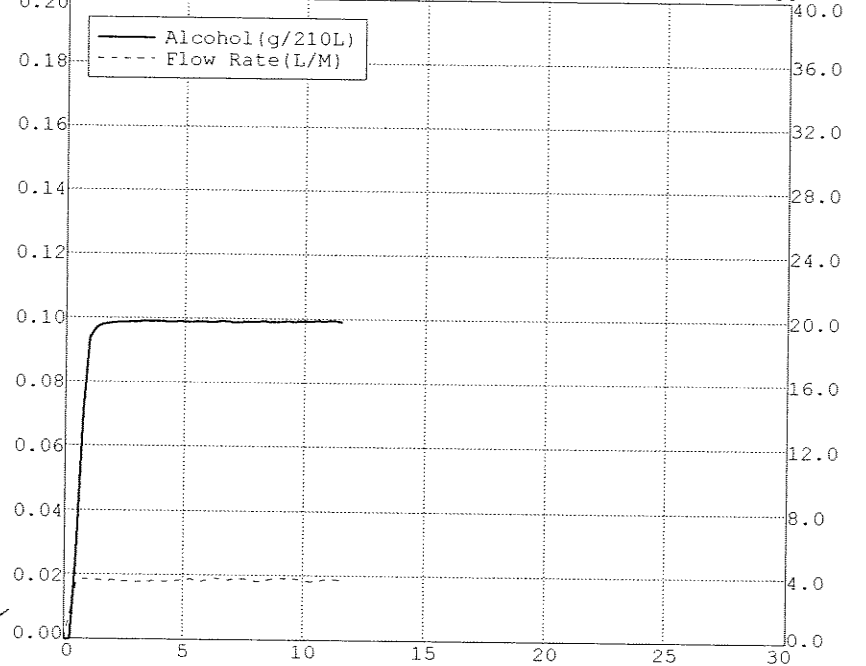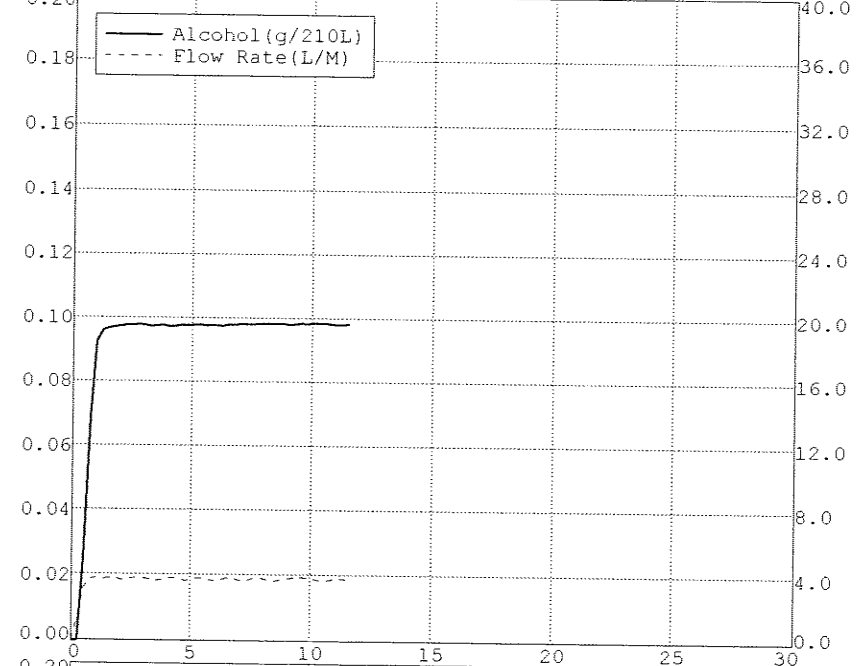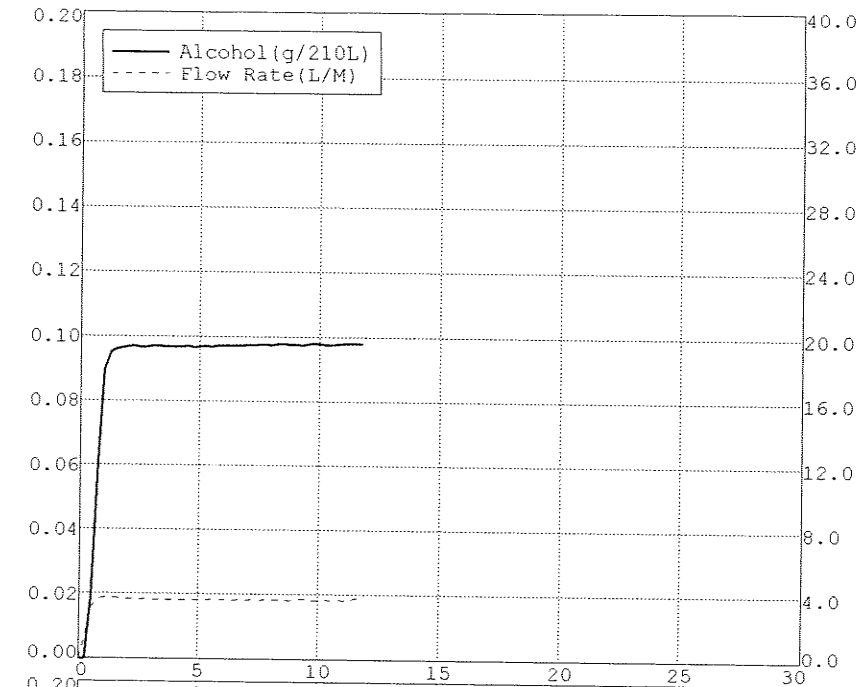

Handwritten signatures and initials:
C. B. Geisler
#20340