

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 10/20/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:24
INTERNAL STANDARD	VERIFIED	16:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:24
BLANK TEST	0.00	16:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:25
BLANK TEST	0.00	16:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:27
BLANK TEST	0.00	16:27

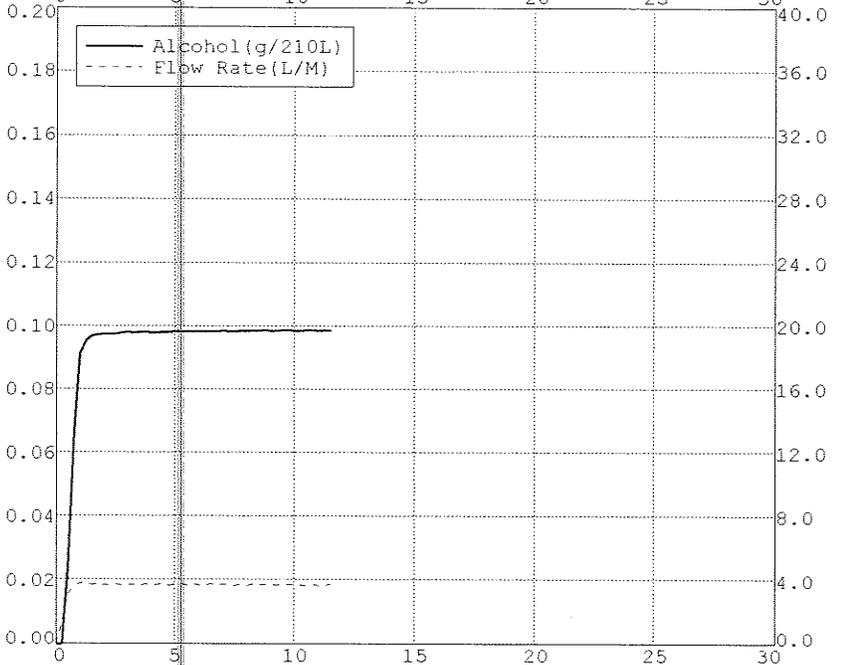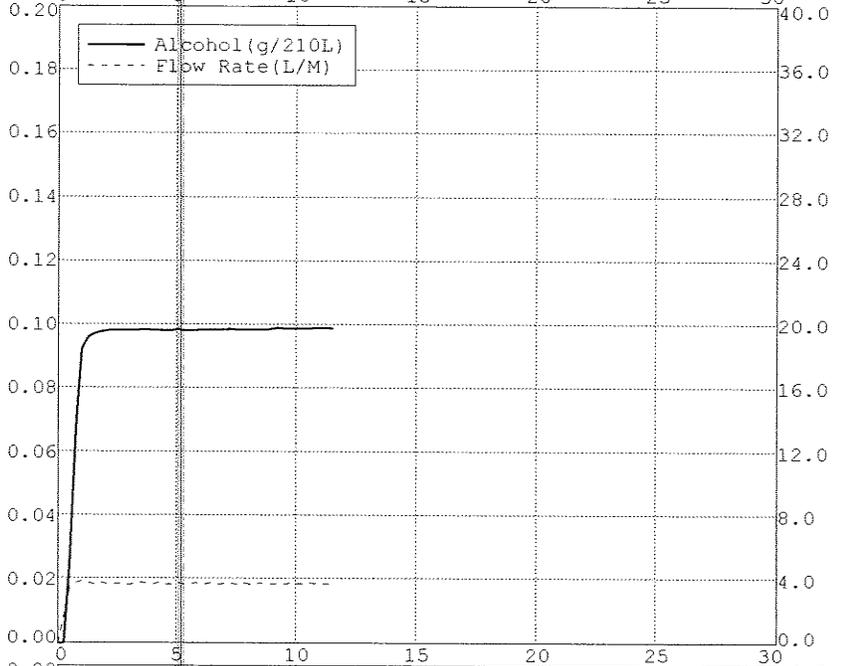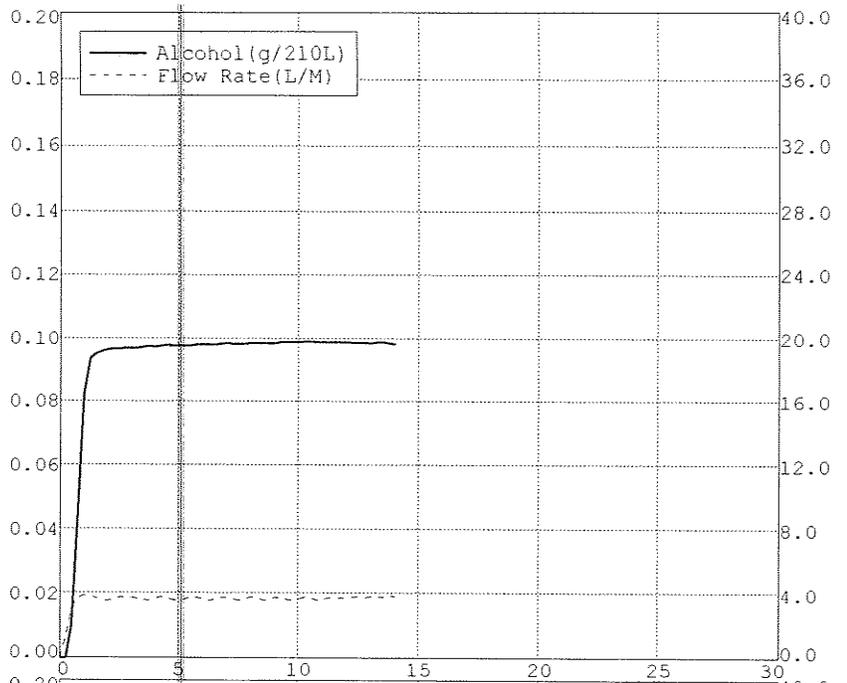

Charles B. Geisler
[Signature]