

SOLUTION CHANGE




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 12/01/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:54
INTERNAL STANDARD	VERIFIED	17:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:54
BLANK TEST	0.00	17:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:56
BLANK TEST	0.00	17:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:57
BLANK TEST	0.00	17:58

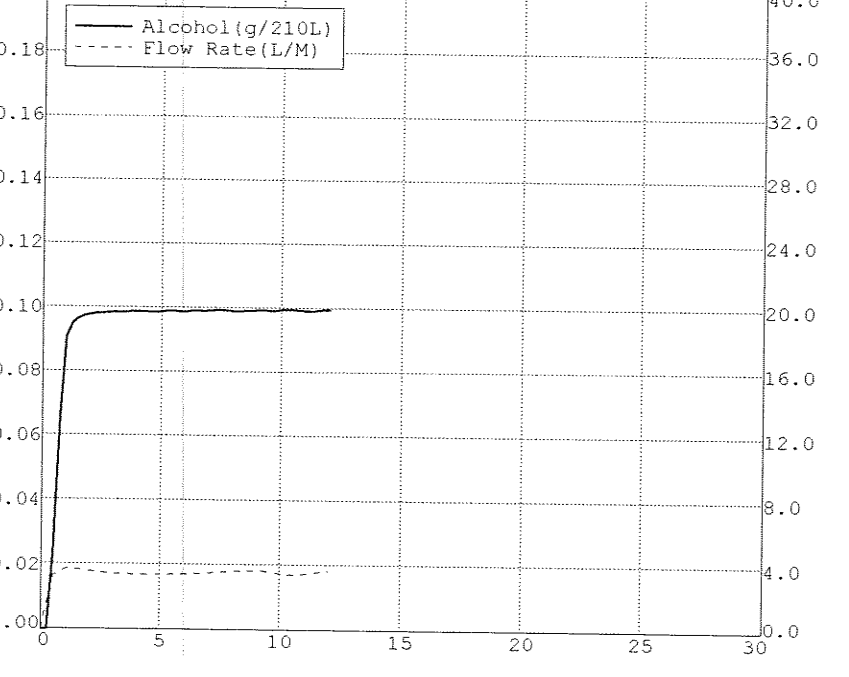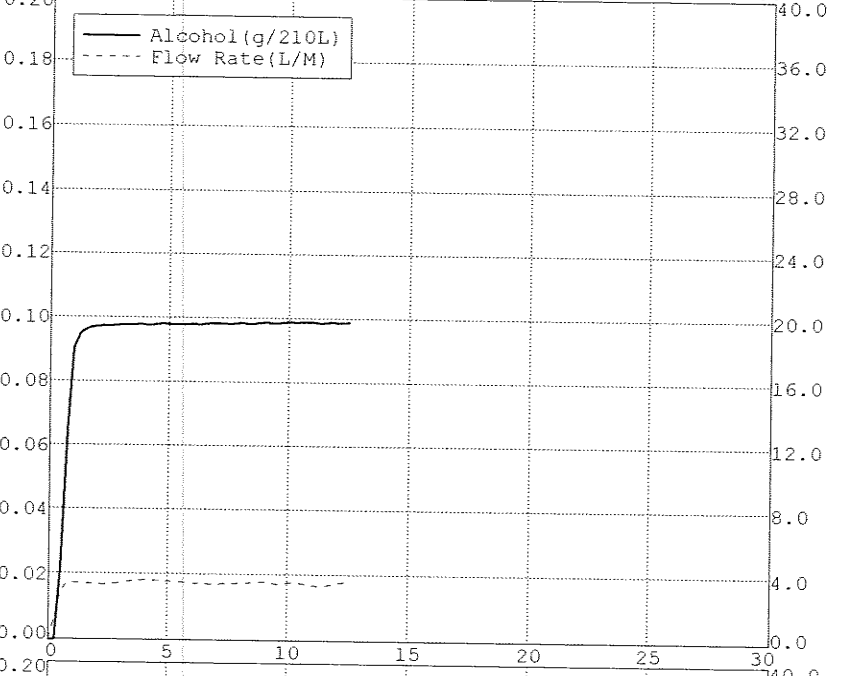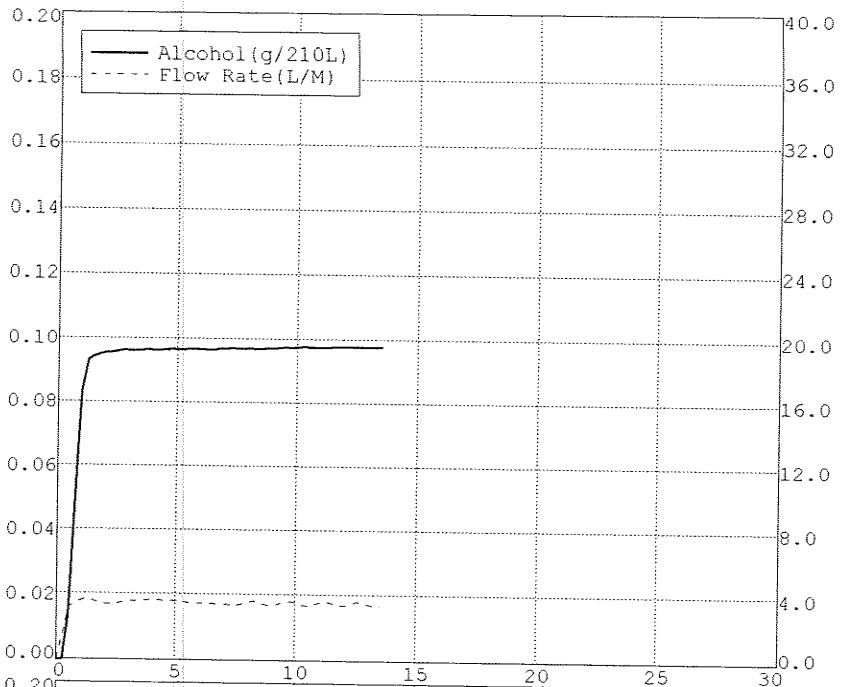

*Charles B Geisler* #20