

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 12/06/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:14
INTERNAL STANDARD	VERIFIED	14:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:15
BLANK TEST	0.00	14:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:16
BLANK TEST	0.00	14:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:17
BLANK TEST	0.00	14:18

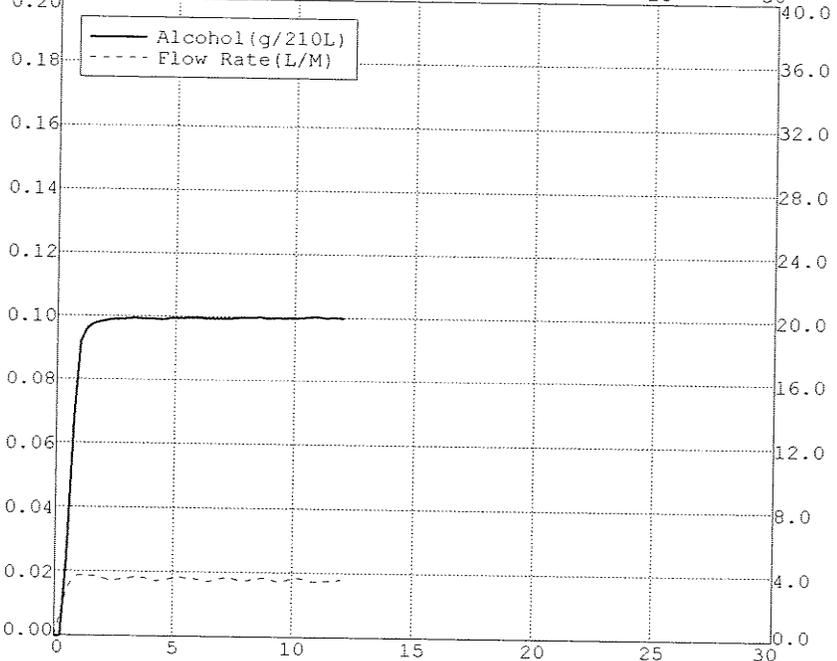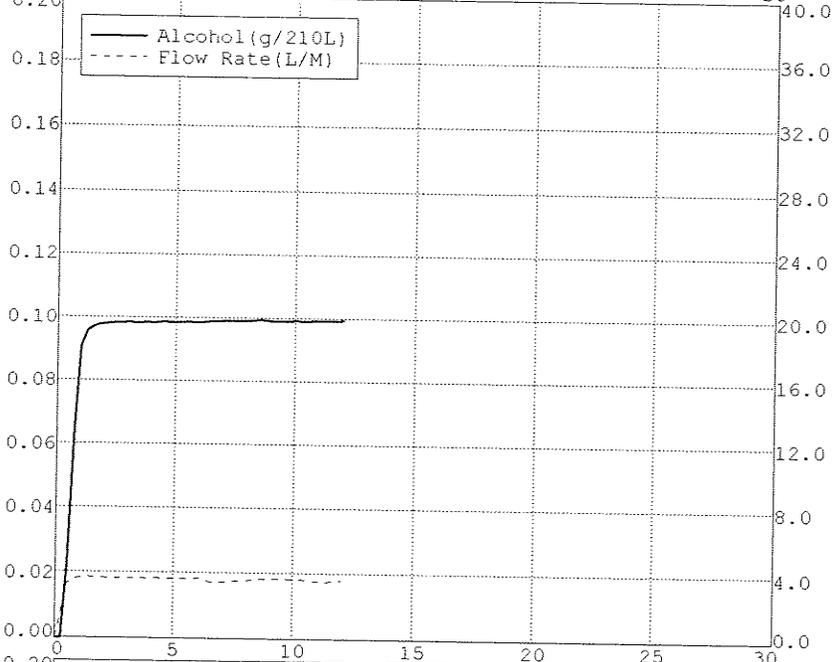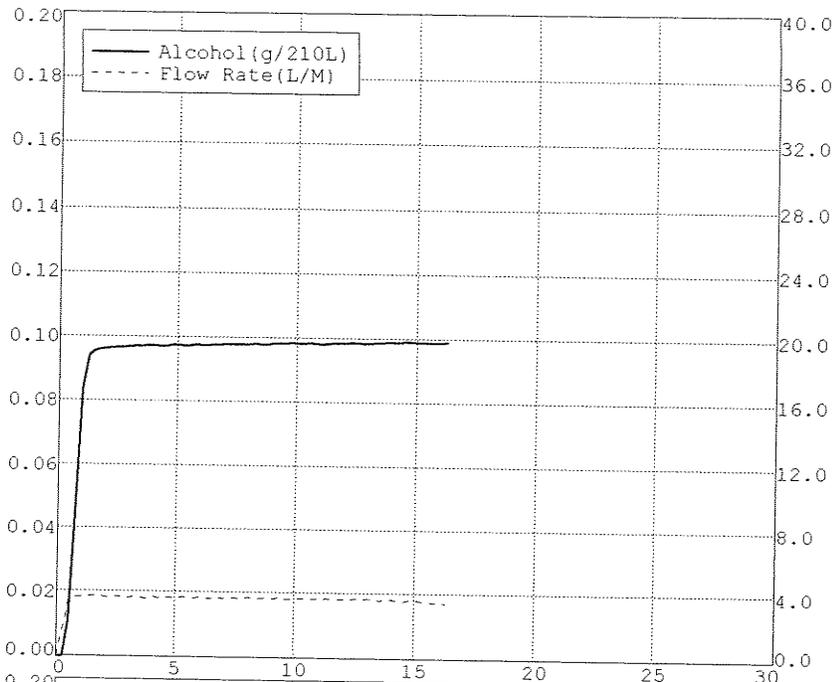

*Charles B. Geisler*