

SUPERVISOR TEST




WARREN COUNTY  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 12/14/2020

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:03
INTERNAL STANDARD	VERIFIED	16:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:04
BLANK TEST	0.00	16:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:05
BLANK TEST	0.00	16:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:06
BLANK TEST	0.00	16:07

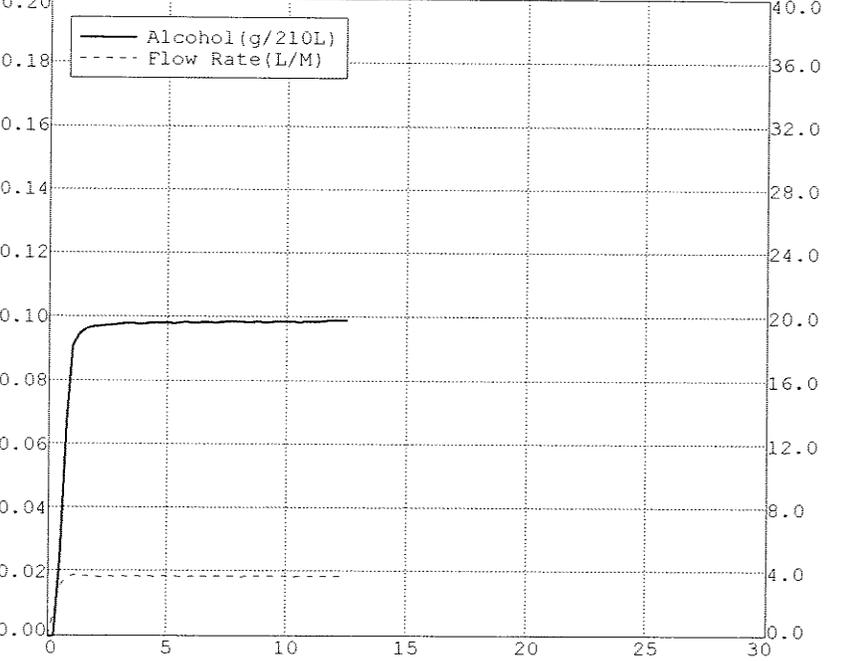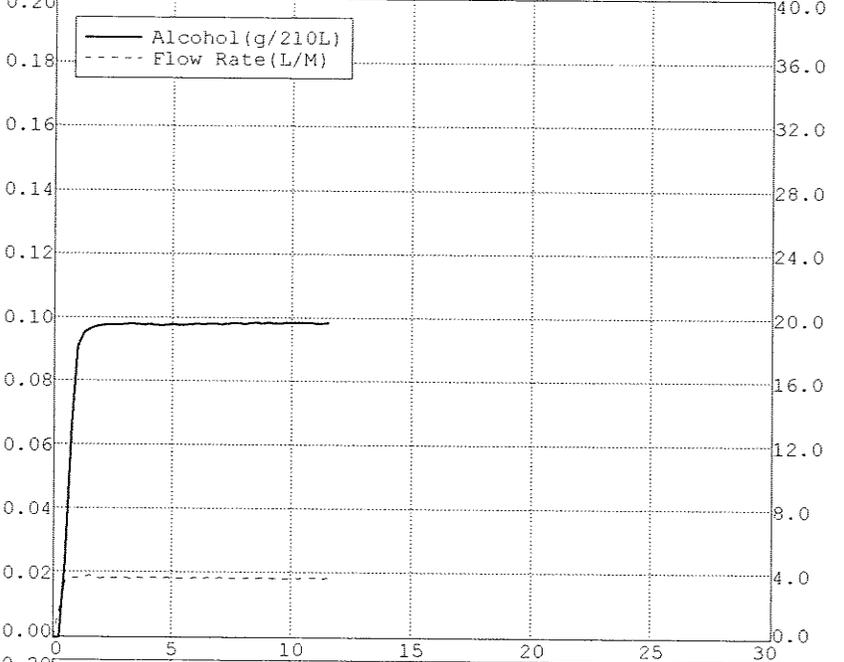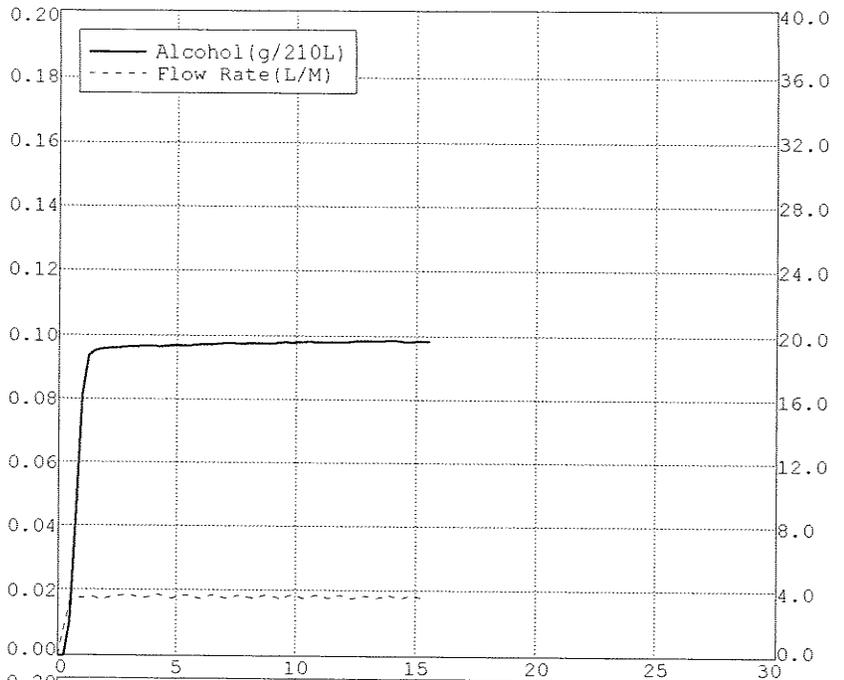

*[Handwritten signatures and initials]*  
 #242