

SUPERVISOR TEST



WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/20/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:53
INTERNAL STANDARD	VERIFIED	14:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:53
BLANK TEST	0.00	14:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:54
BLANK TEST	0.00	14:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:55
BLANK TEST	0.00	14:56

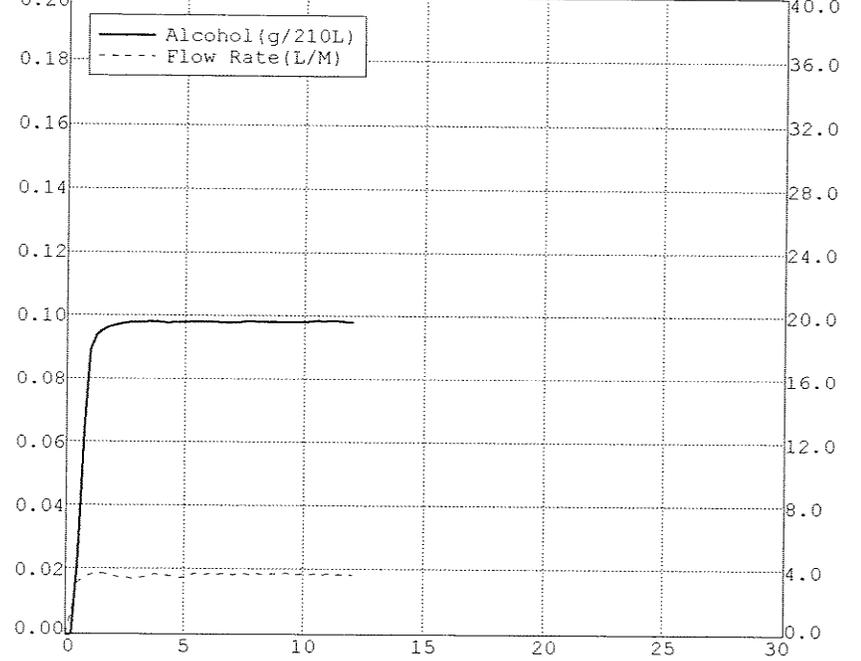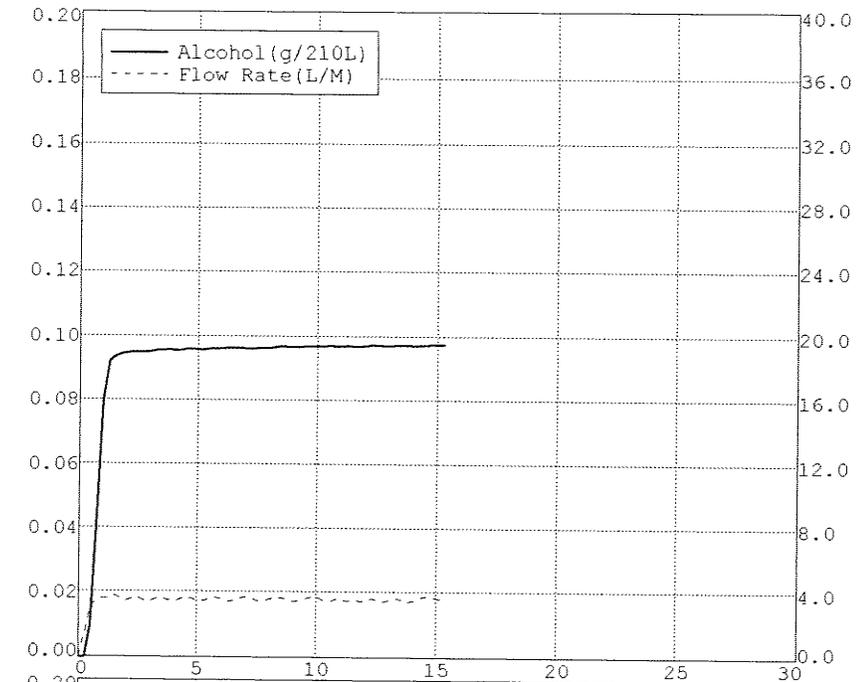

Charles B. Geisler #248