

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/28/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:39
INTERNAL STANDARD	VERIFIED	15:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:40
BLANK TEST	0.00	15:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:41
BLANK TEST	0.00	15:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:42
BLANK TEST	0.00	15:43

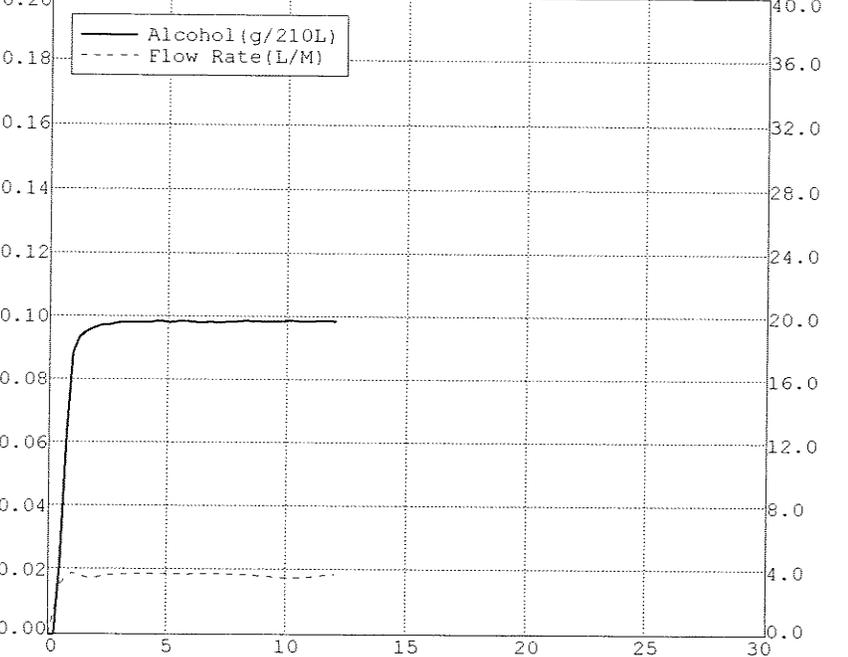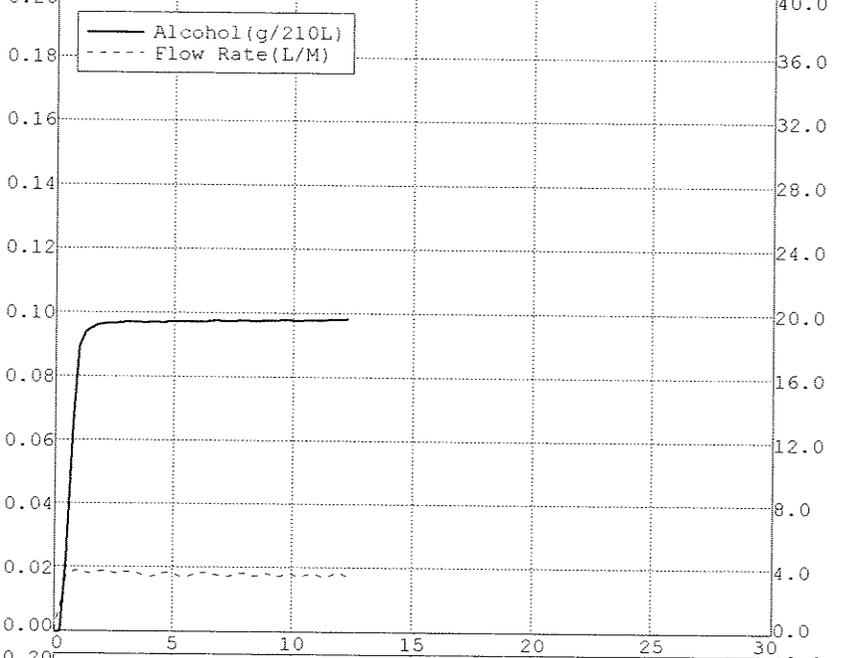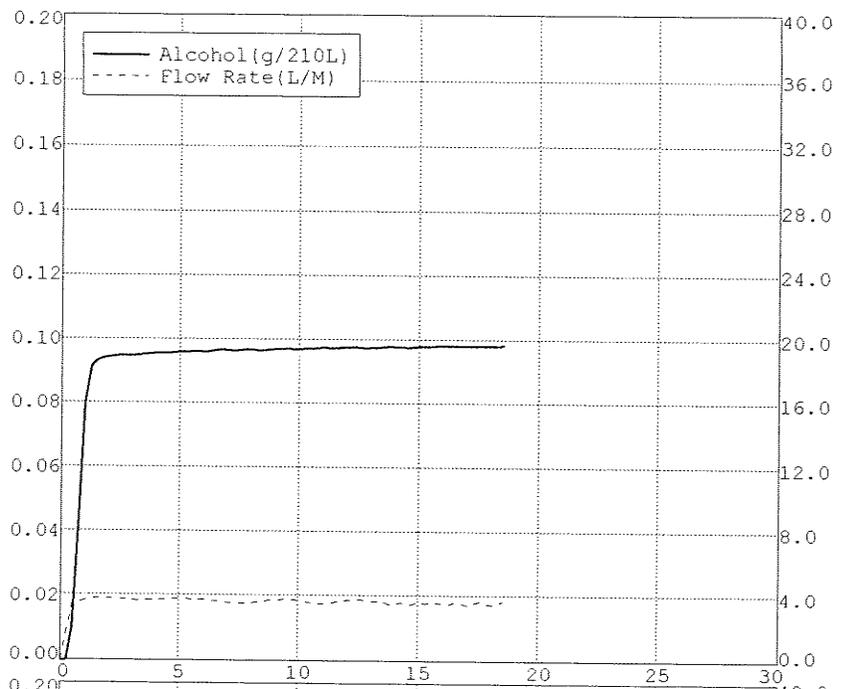

Charles B. Geisler #241