

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 01/29/2021

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:16
INTERNAL STANDARD	VERIFIED	16:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:16
BLANK TEST	0.00	16:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:17
BLANK TEST	0.00	16:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:18
BLANK TEST	0.00	16:19

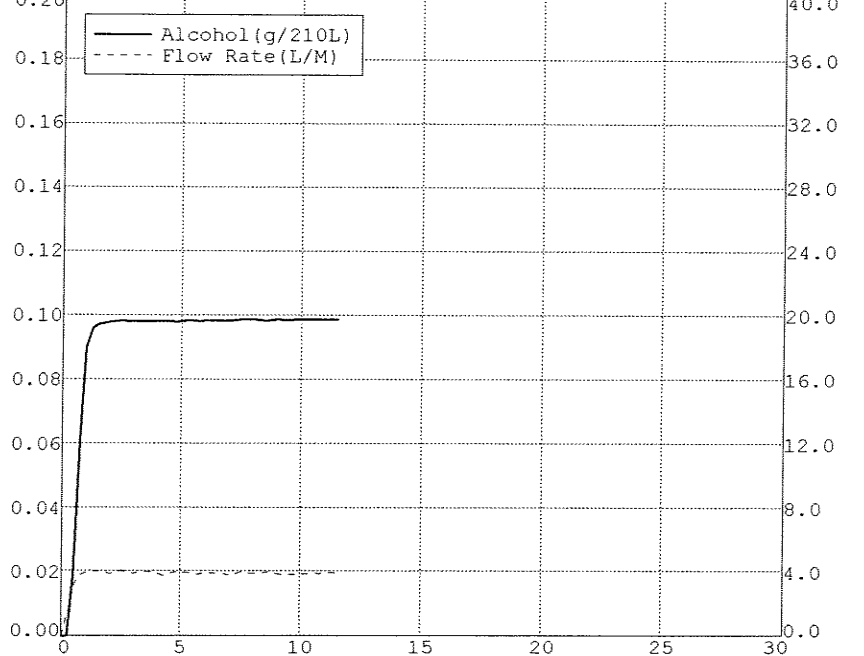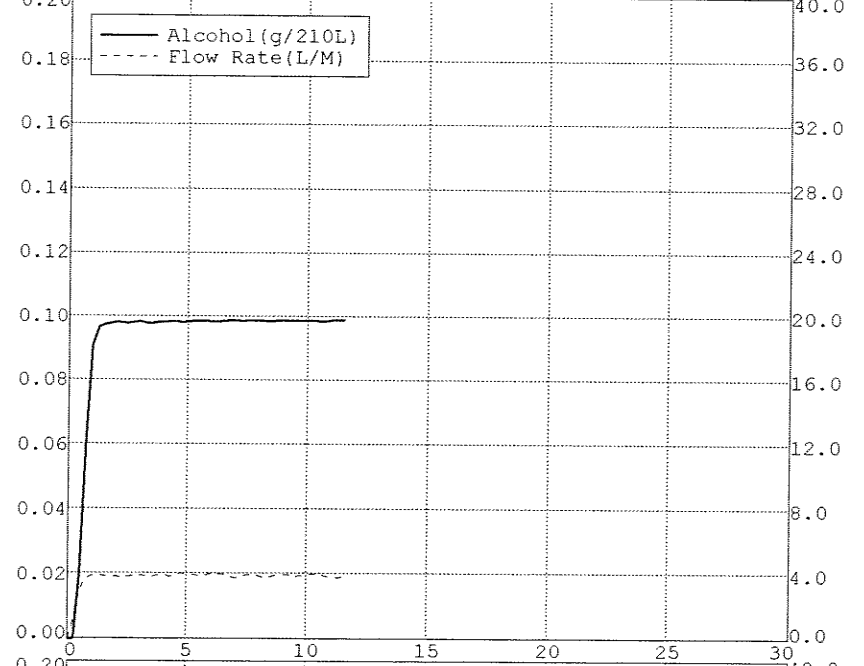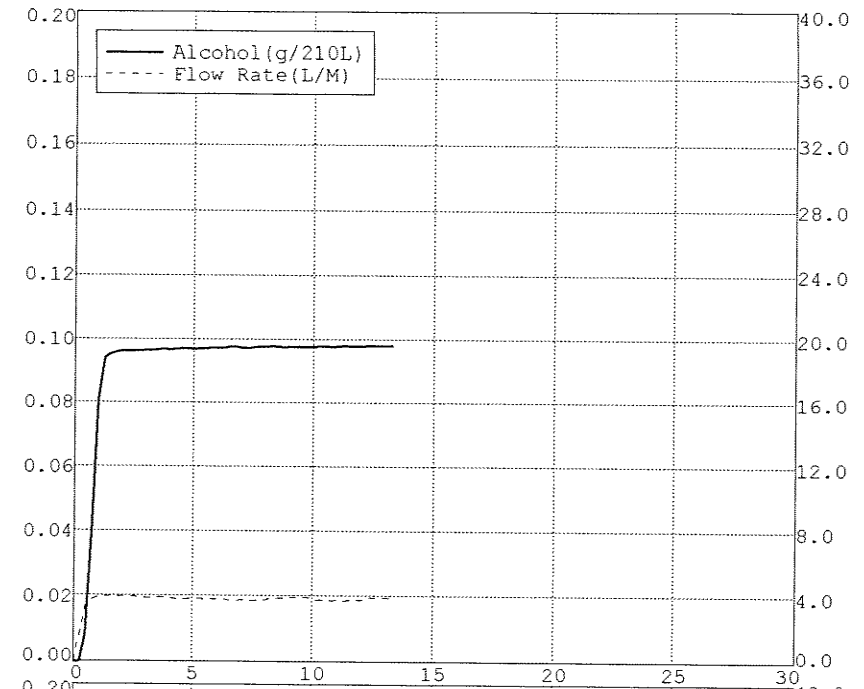

*Sgt. C. B. Geisler*      *[Signature]*