

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 02/22/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:38
INTERNAL STANDARD	VERIFIED	11:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:39
BLANK TEST	0.00	11:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:40
BLANK TEST	0.00	11:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:41
BLANK TEST	0.00	11:42

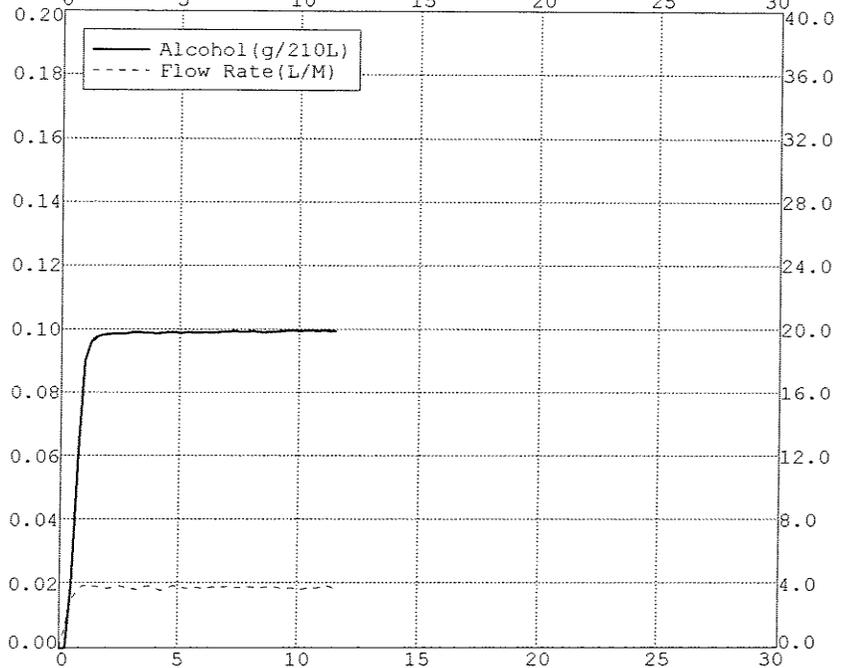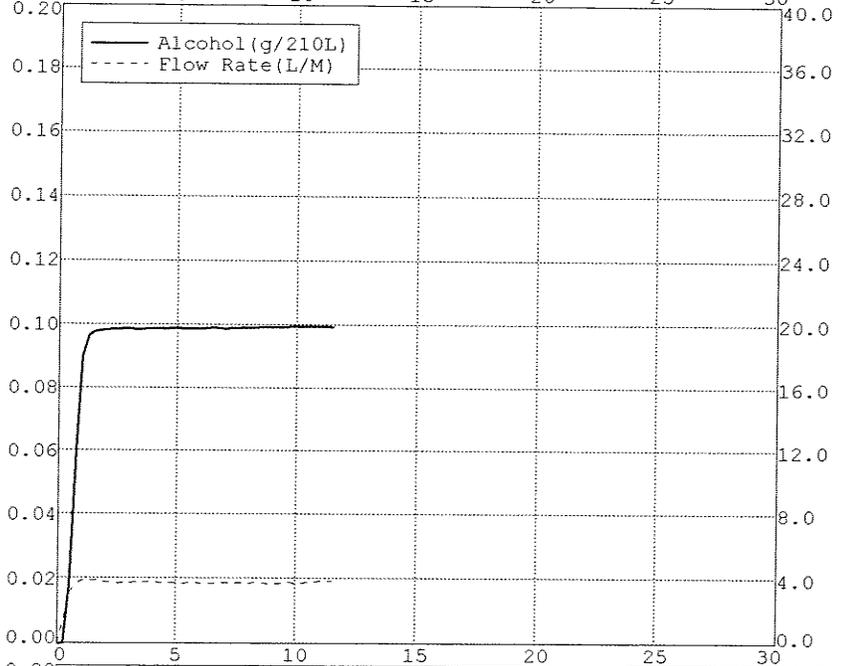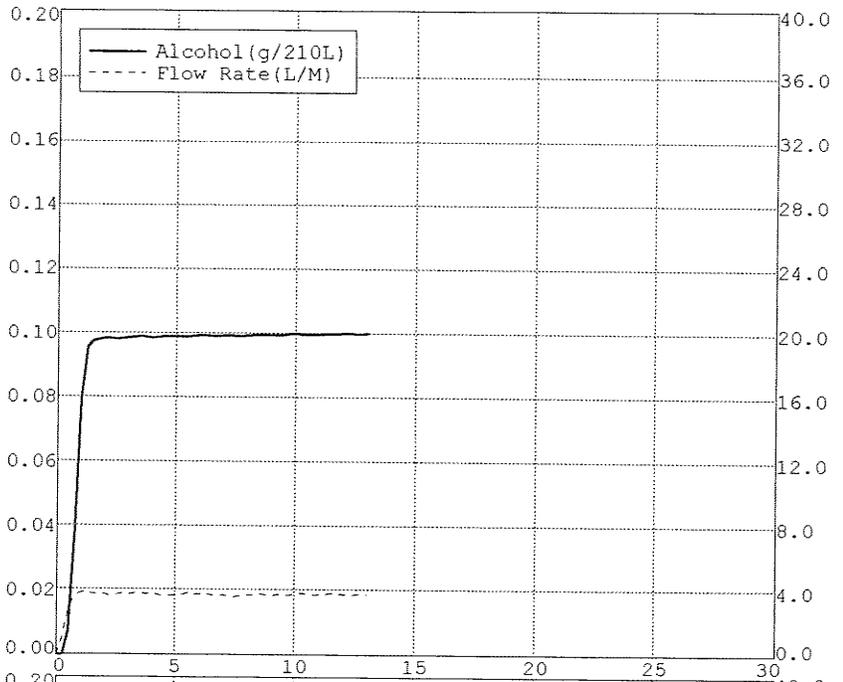

Handwritten signatures and initials:
C. B. Geisler
M. J. [unclear]
#204