

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/28/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:45
INTERNAL STANDARD	VERIFIED	10:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:46
BLANK TEST	0.00	10:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:47
BLANK TEST	0.00	10:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:48
BLANK TEST	0.00	10:49

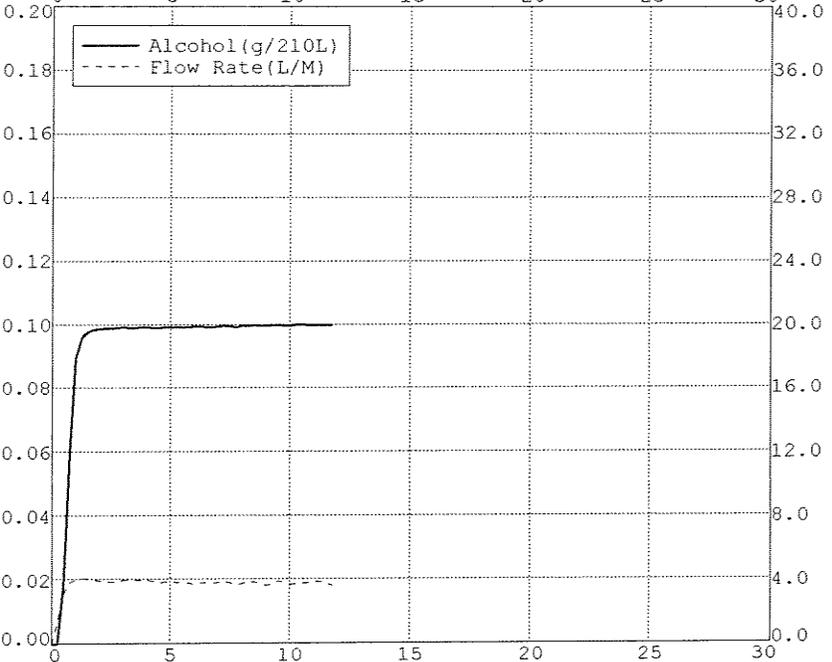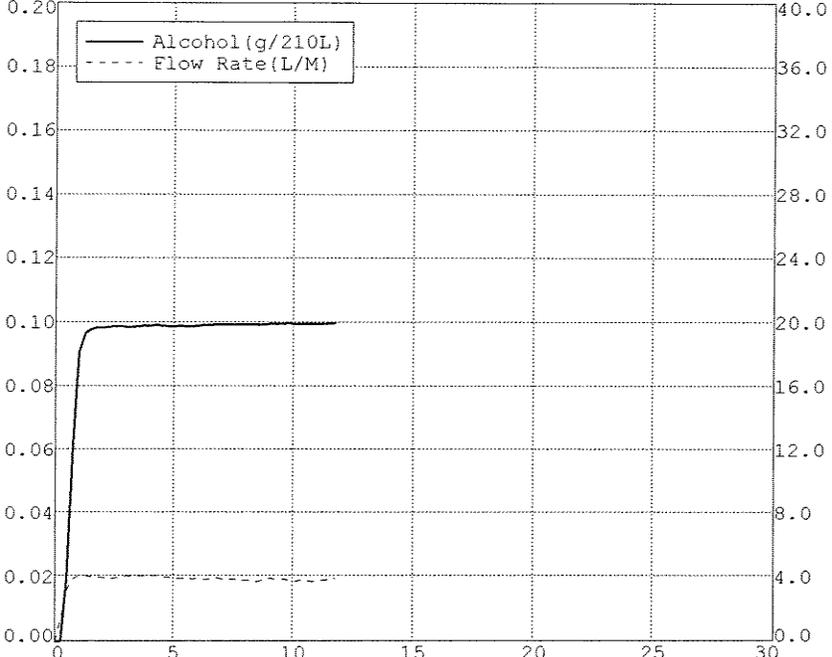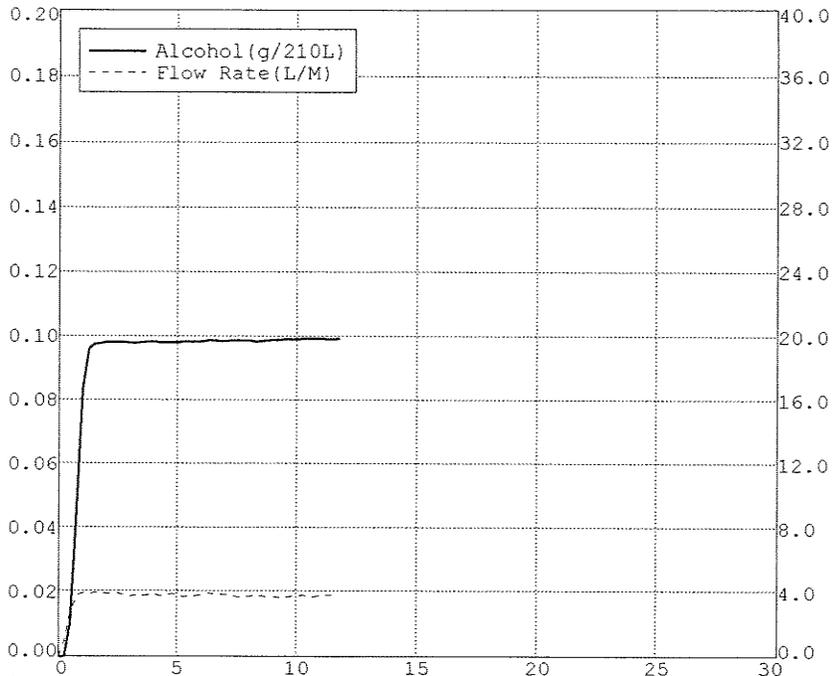

*Charles B Geisler* #244