

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 03/14/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:24
INTERNAL STANDARD	VERIFIED	13:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:24
BLANK TEST	0.00	13:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:25
BLANK TEST	0.00	13:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:26
BLANK TEST	0.00	13:27

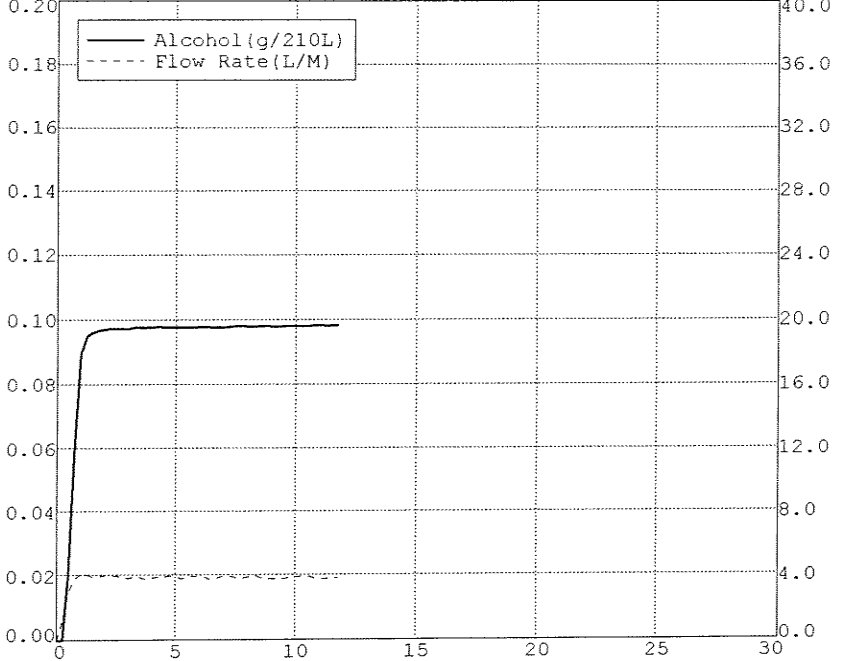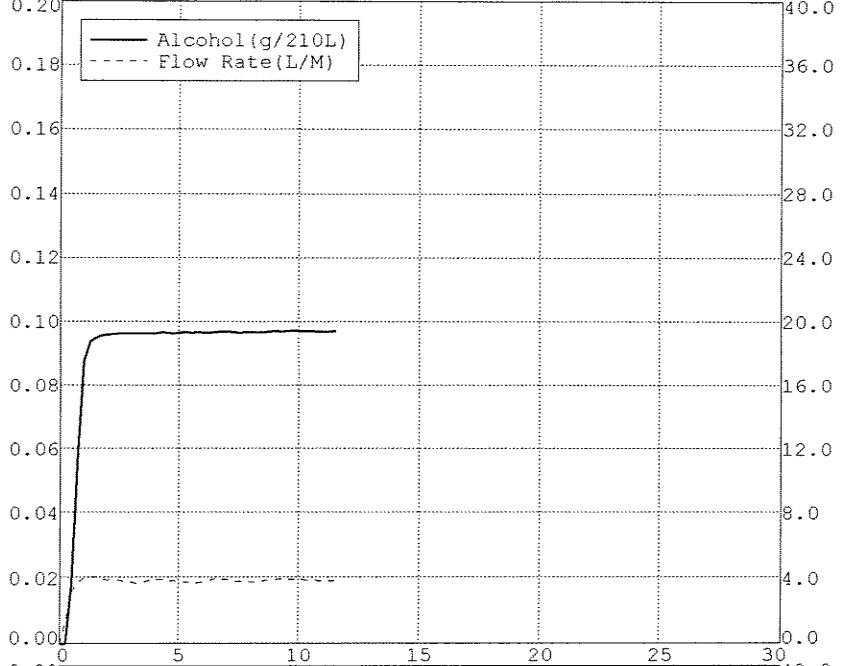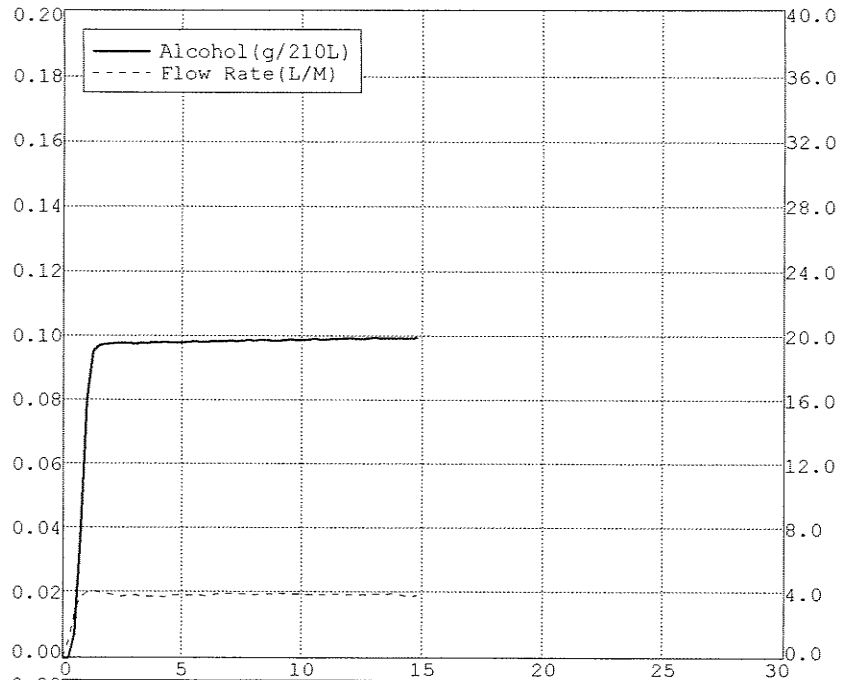

*Sgt. Charles B. Geisler*