

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/17/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:24
INTERNAL STANDARD	VERIFIED	13:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:24
BLANK TEST	0.00	13:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:25
BLANK TEST	0.00	13:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:27
BLANK TEST	0.00	13:27

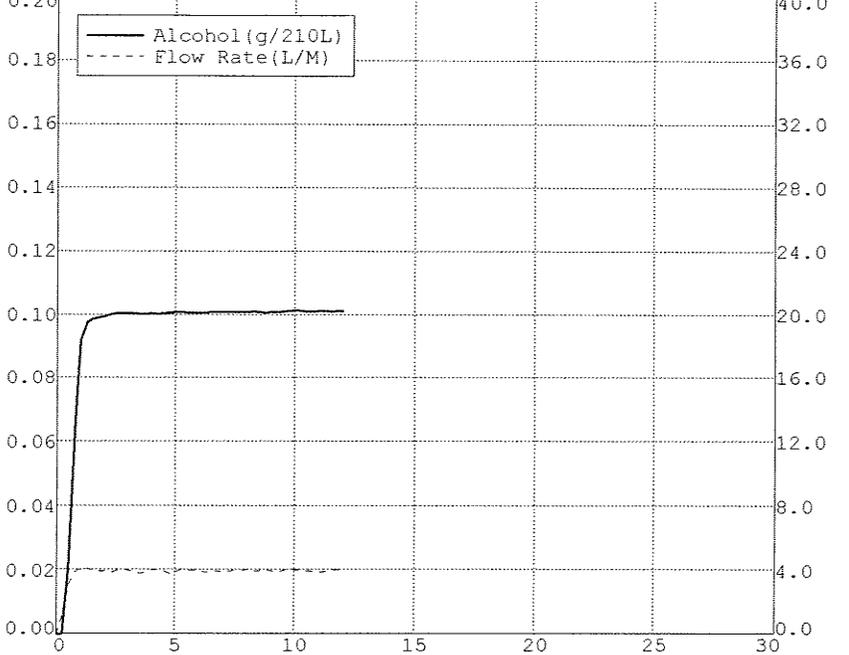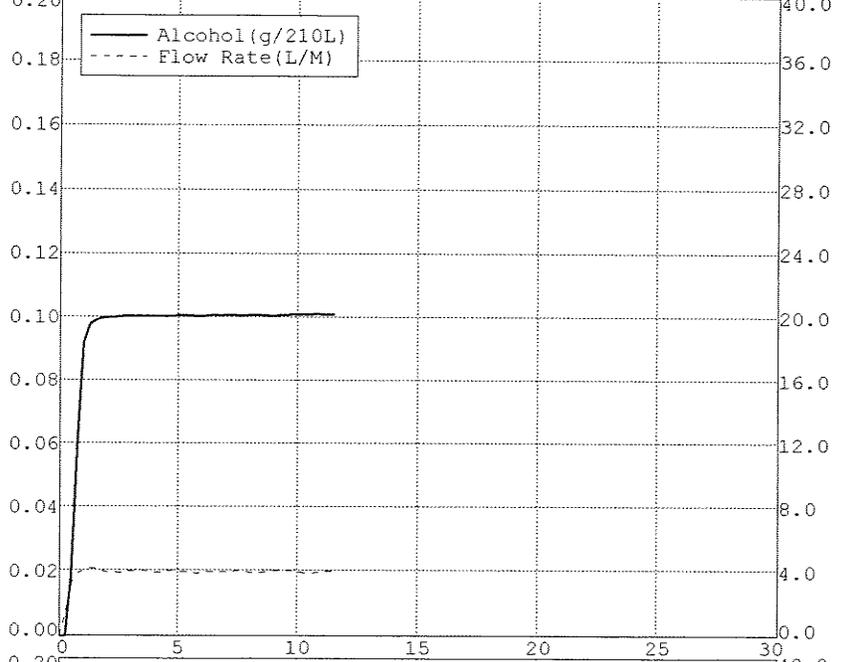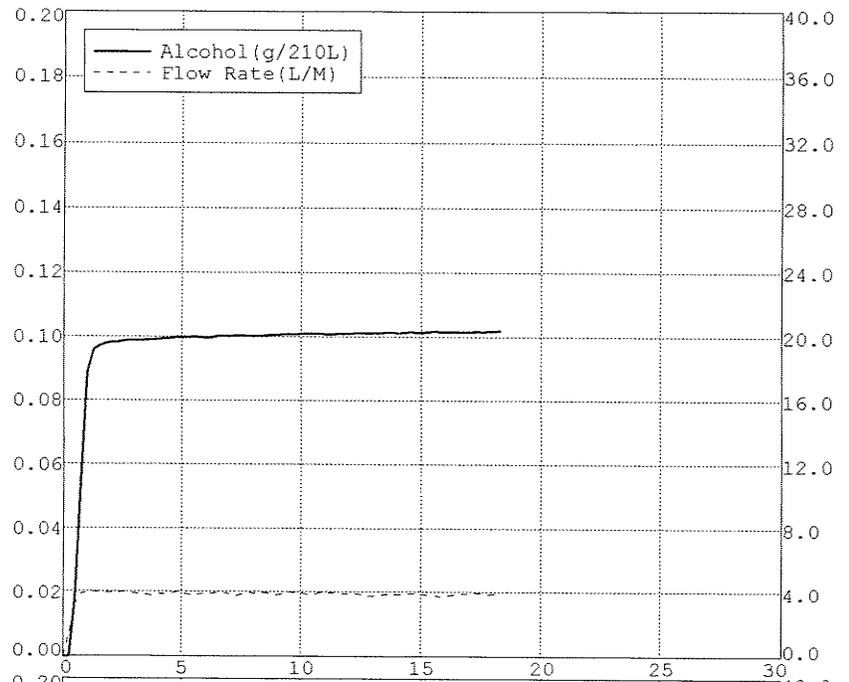

Handwritten signature and initials