

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/01/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:44
INTERNAL STANDARD	VERIFIED	13:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:44
BLANK TEST	0.00	13:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:45
BLANK TEST	0.00	13:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:47
BLANK TEST	0.00	13:48

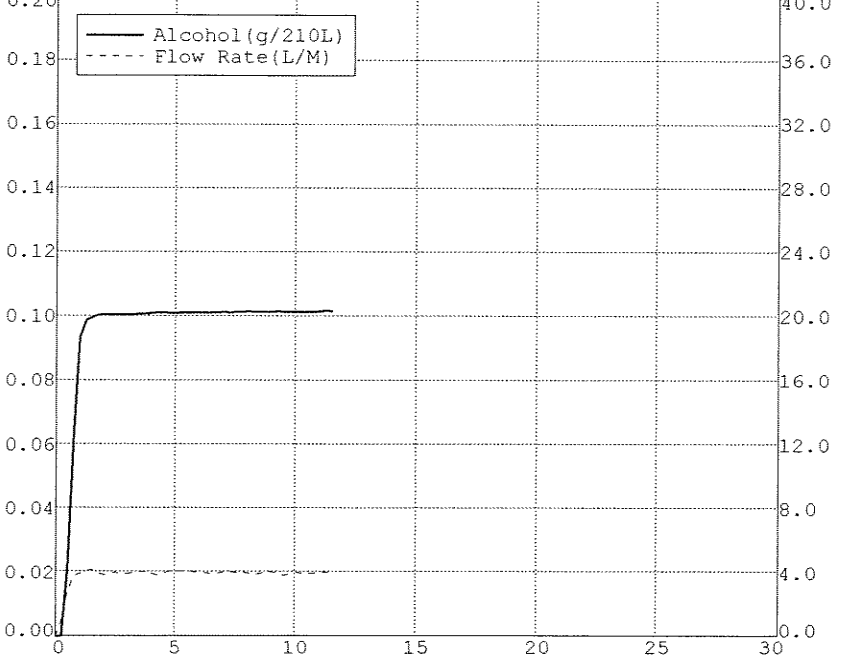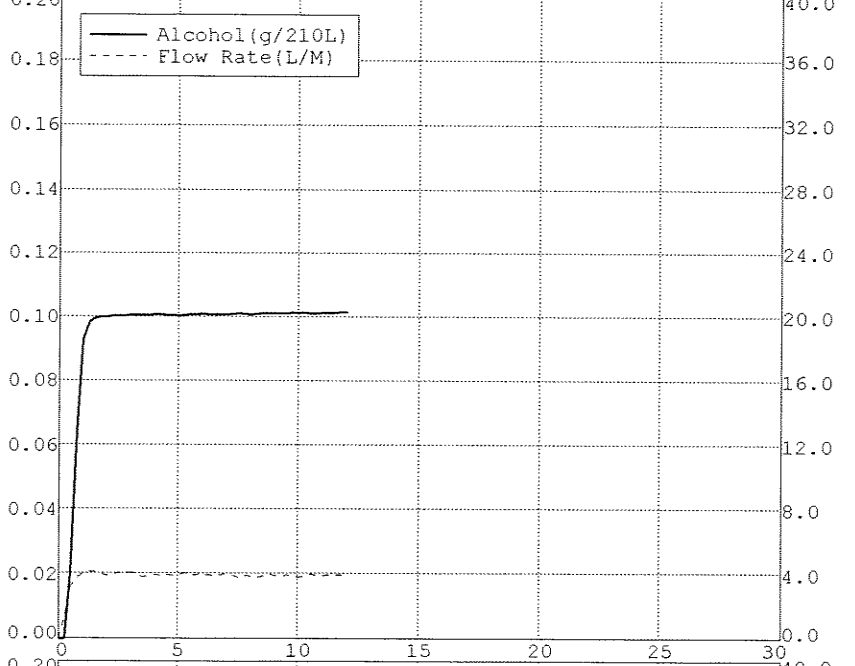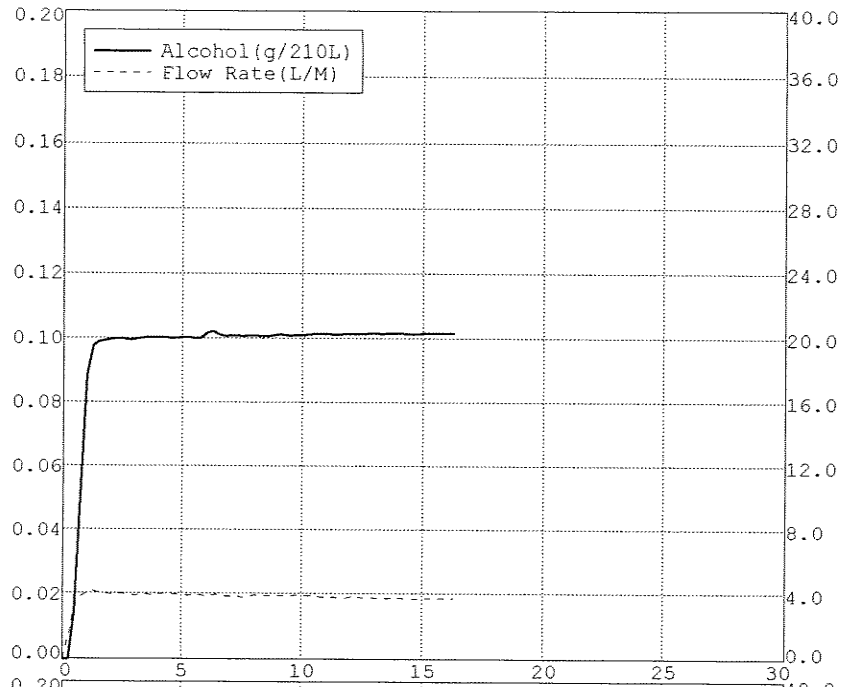

Charles B. Geisler #241