

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 06/14/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:04
INTERNAL STANDARD	VERIFIED	16:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:05
BLANK TEST	0.00	16:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:06
BLANK TEST	0.00	16:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:07
BLANK TEST	0.00	16:08

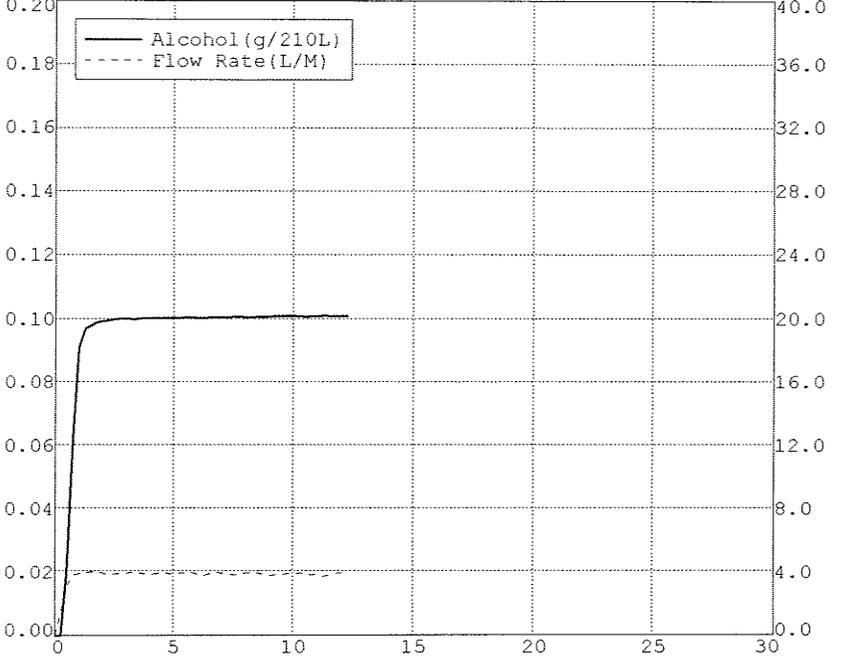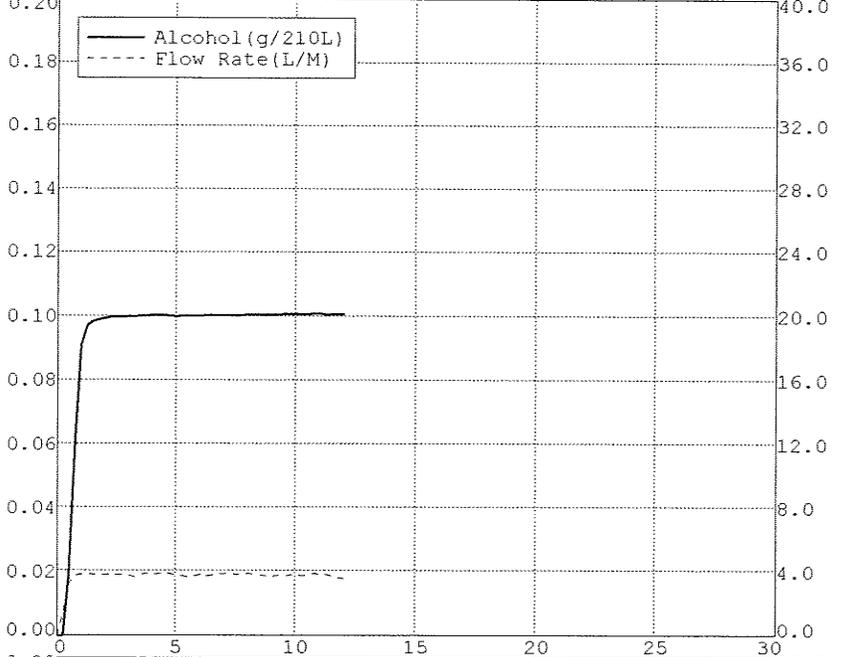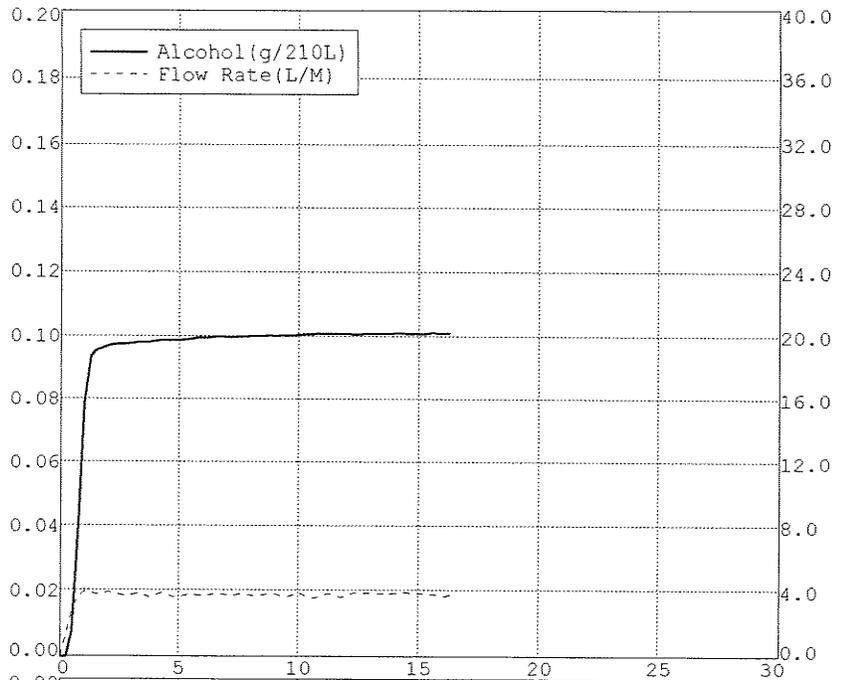

*Signature: Sgt. Charles B. Geisler*