

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/20/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:20
INTERNAL STANDARD	VERIFIED	11:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:21
BLANK TEST	0.00	11:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:22
BLANK TEST	0.00	11:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:23
BLANK TEST	0.00	11:24

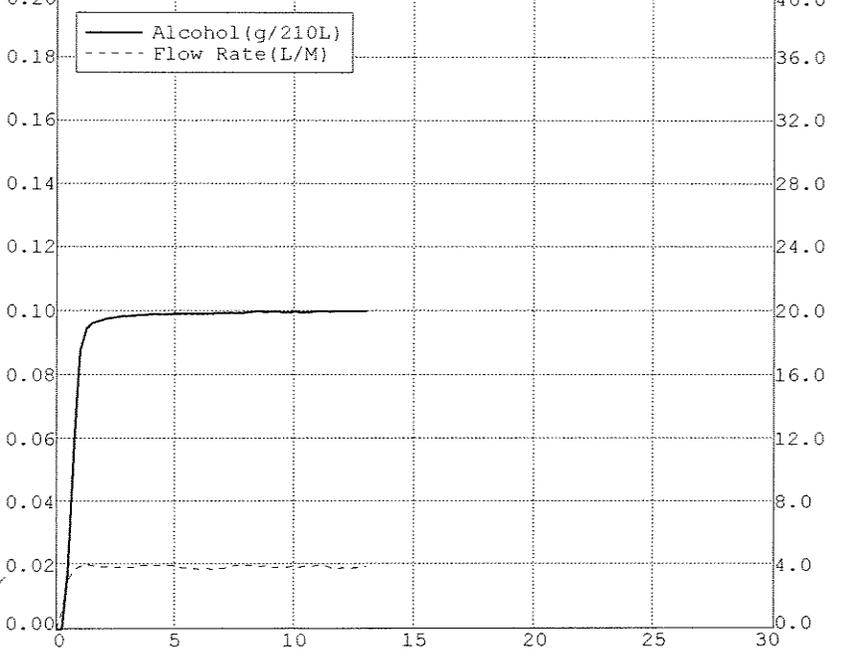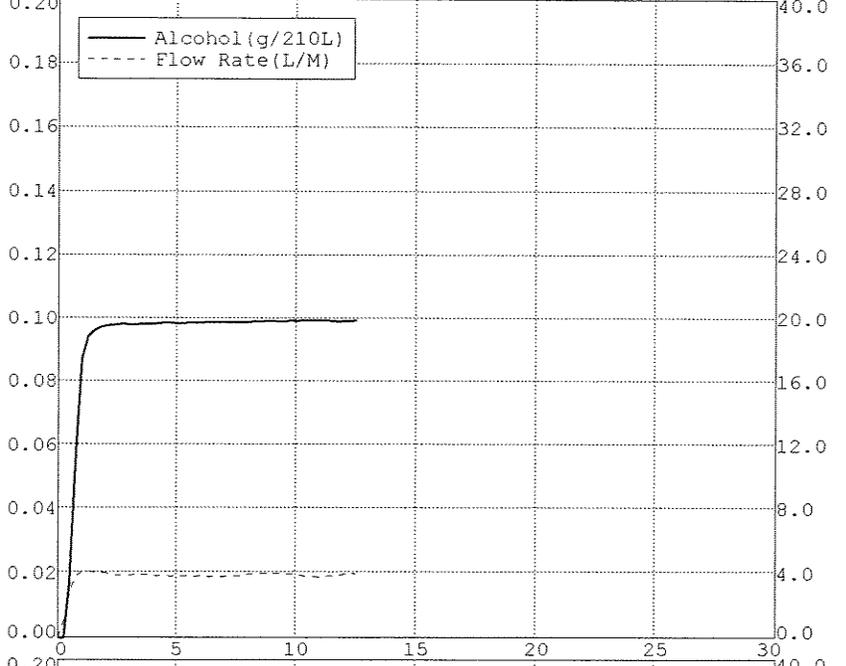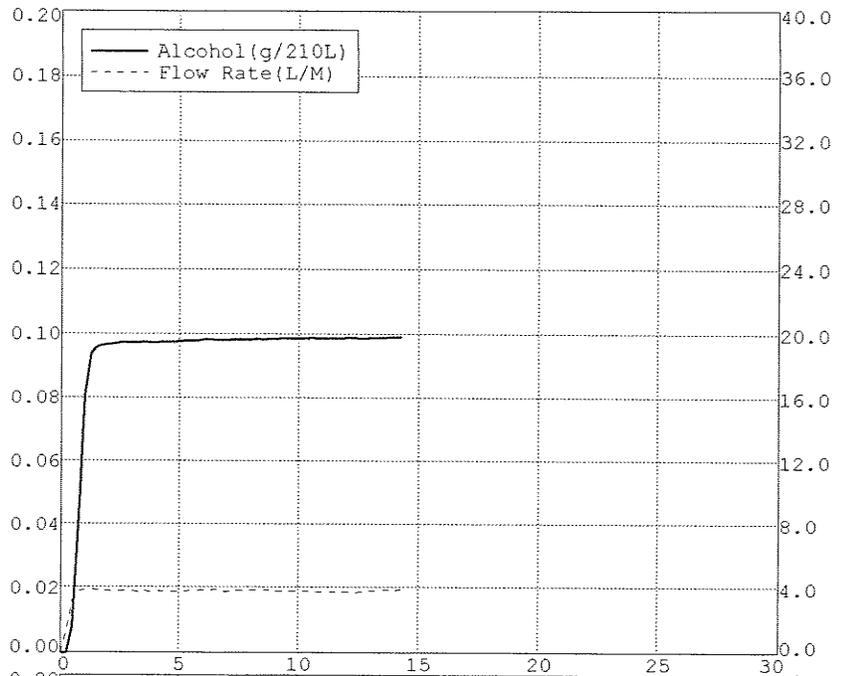

Sgt. Charles B. Geisler