

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/09/2021

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 02:19 |
| INTERNAL STANDARD | VERIFIED | 02:20 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 02:20 |
| BLANK TEST | 0.00 | 02:21 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 02:21 |
| BLANK TEST | 0.00 | 02:22 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 02:22 |
| BLANK TEST | 0.00 | 02:23 |

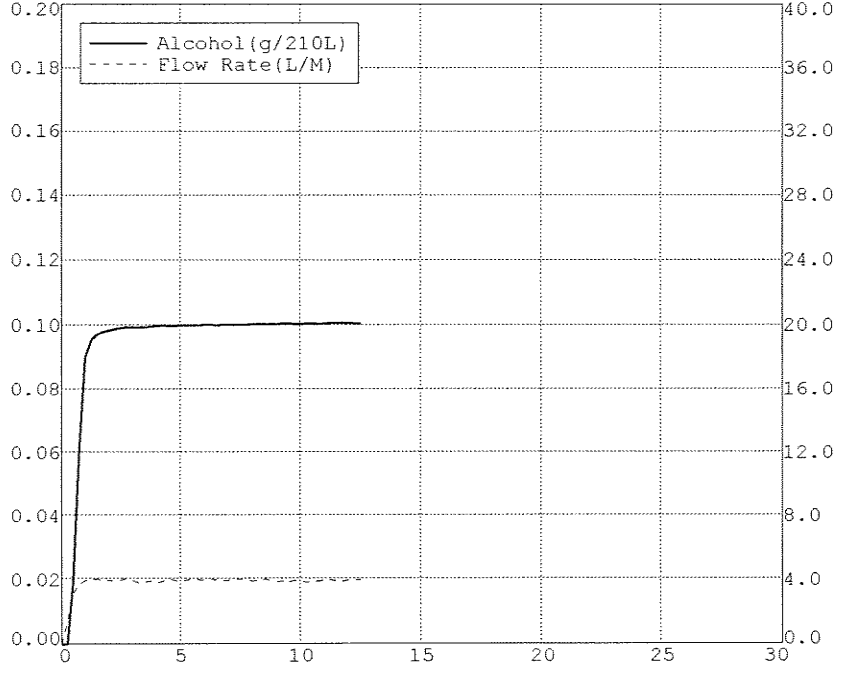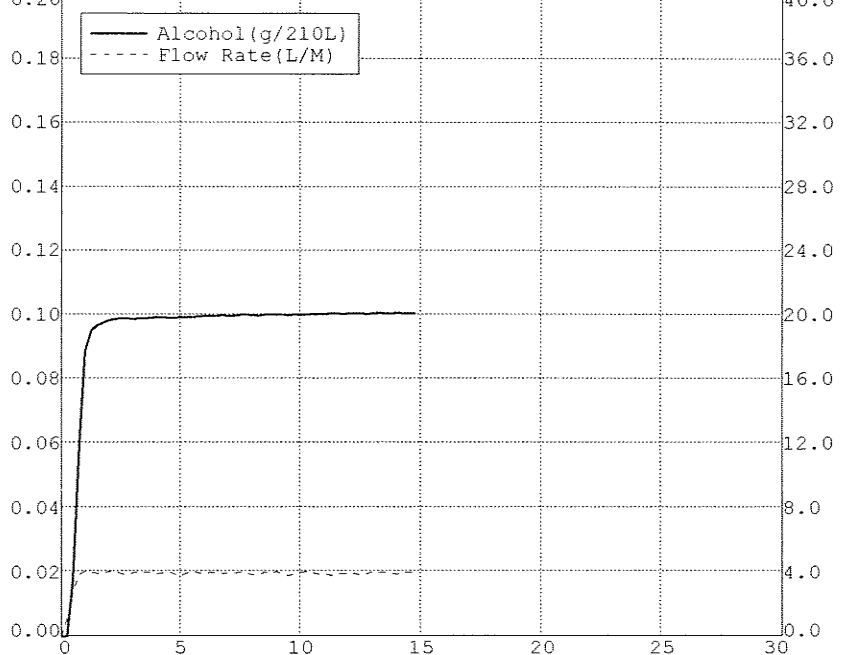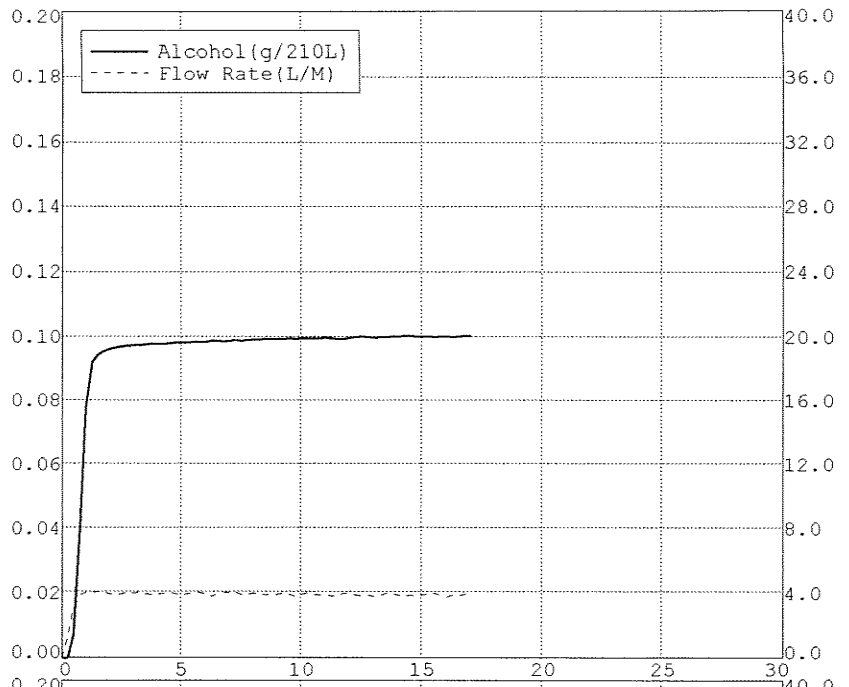

PO M. A. Campbell #157