

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/09/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:21
INTERNAL STANDARD	VERIFIED	13:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:22
BLANK TEST	0.00	13:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:23
BLANK TEST	0.00	13:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:24
BLANK TEST	0.00	13:25

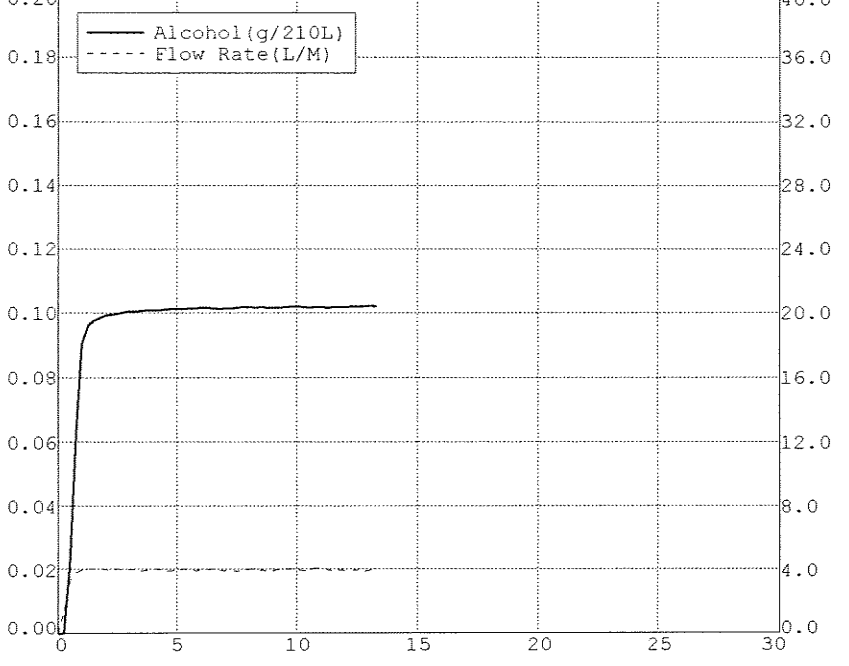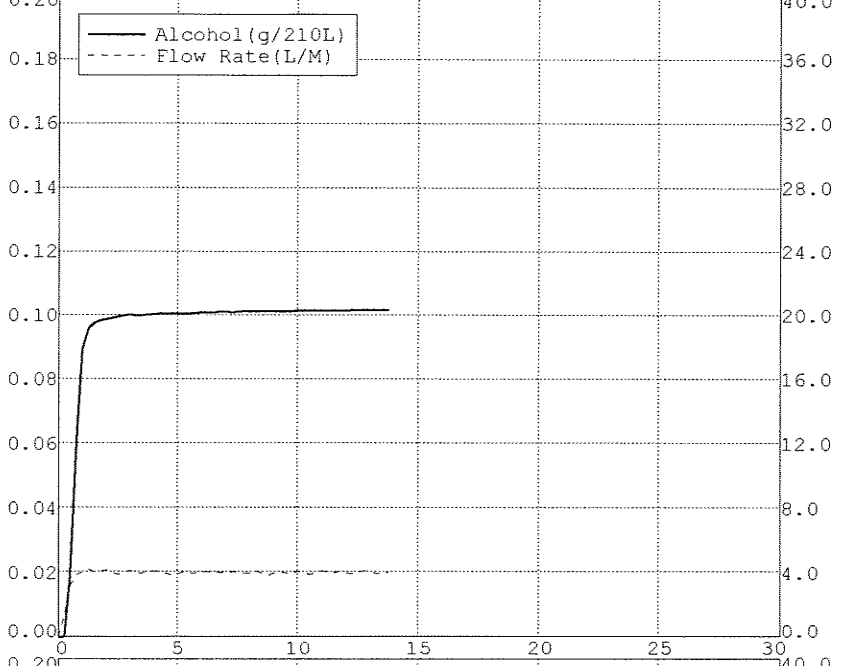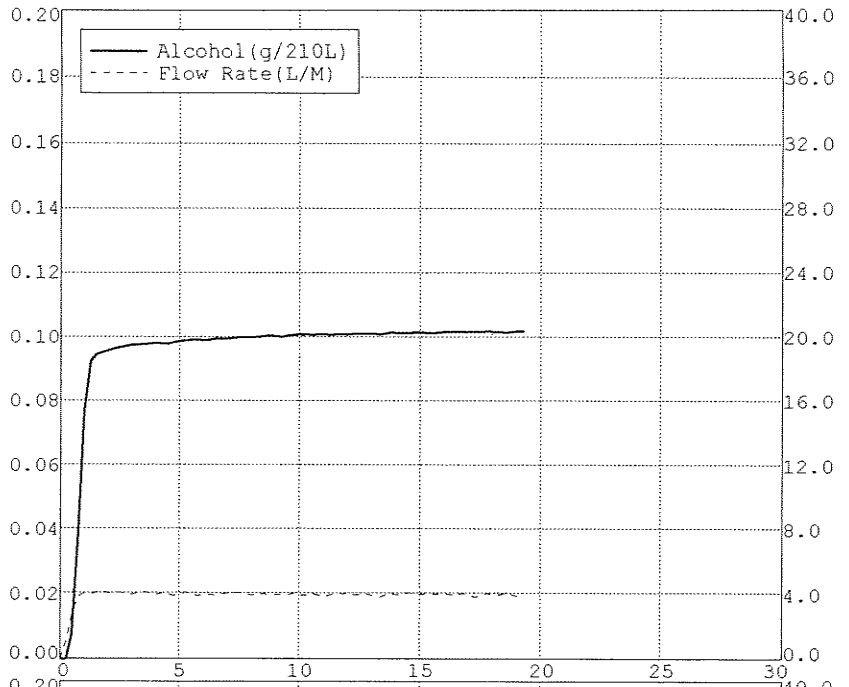

Egt. Chl - 0. *CG* *HW*