

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/23/2021

OPERATOR NAME:
SEAN T SMITH
Permit #: 46227
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:25
INTERNAL STANDARD	VERIFIED	09:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:26
BLANK TEST	0.00	09:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:27
BLANK TEST	0.00	09:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:28
BLANK TEST	0.00	09:29

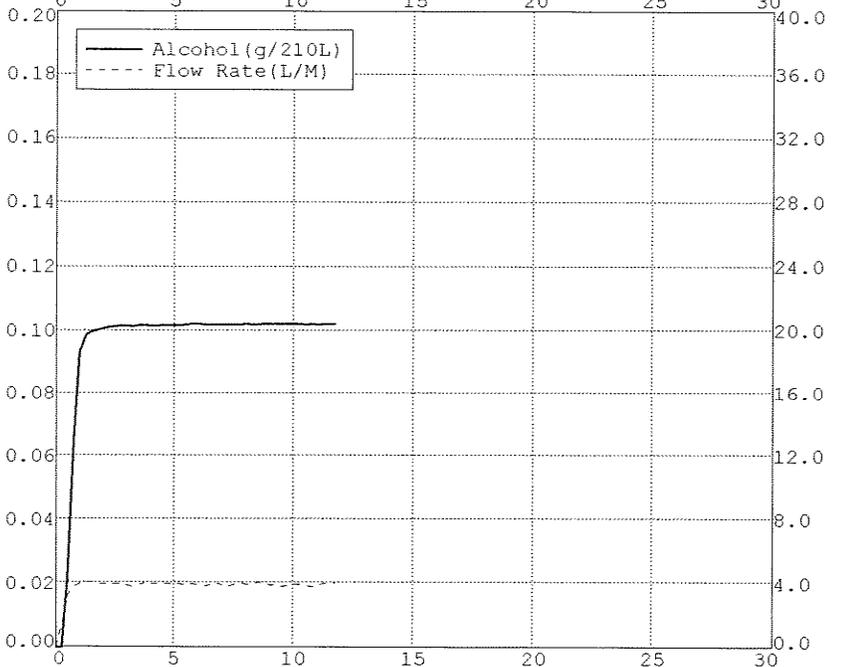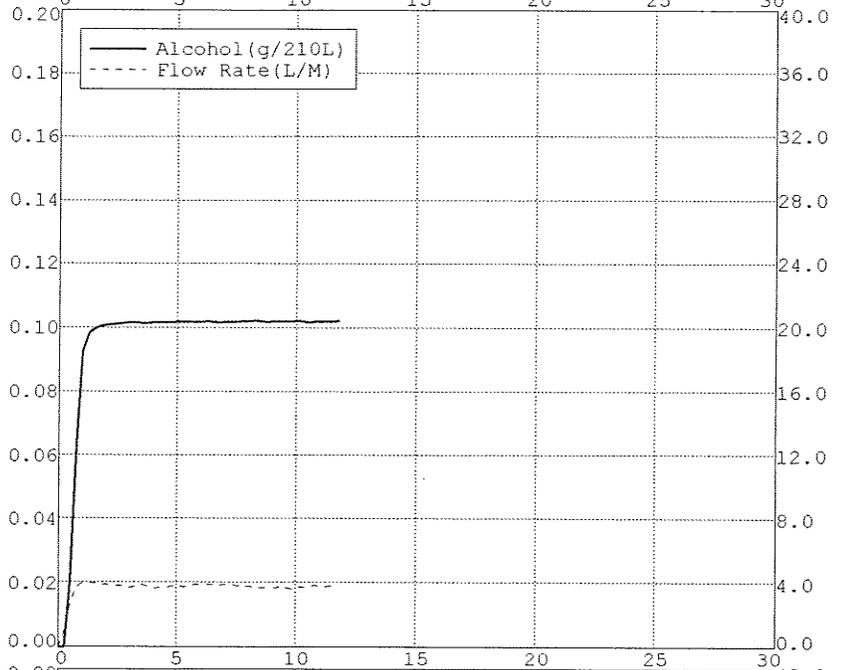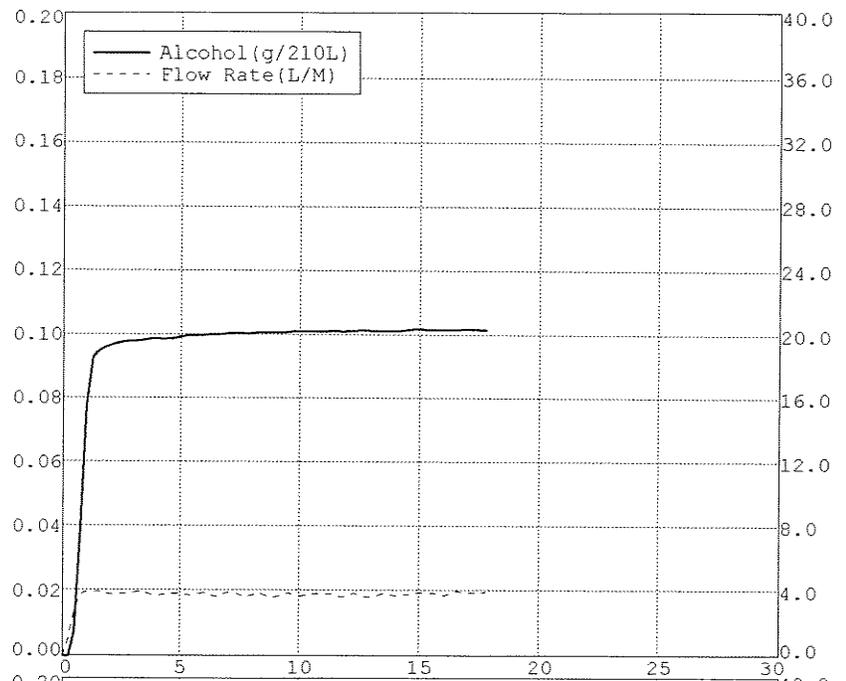

Signature 815