

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/01/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:08
INTERNAL STANDARD	VERIFIED	15:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:09
BLANK TEST	0.00	15:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:11
BLANK TEST	0.00	15:12

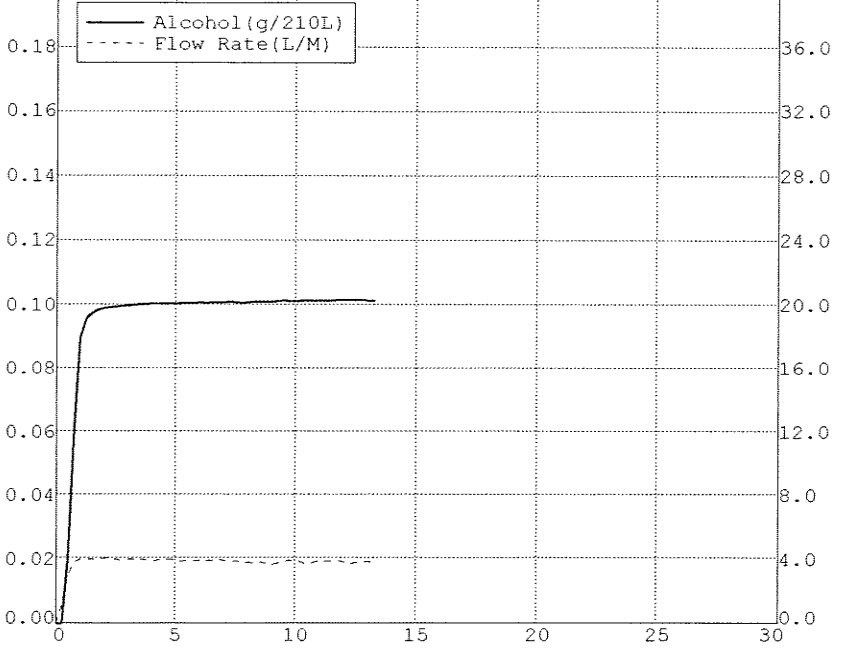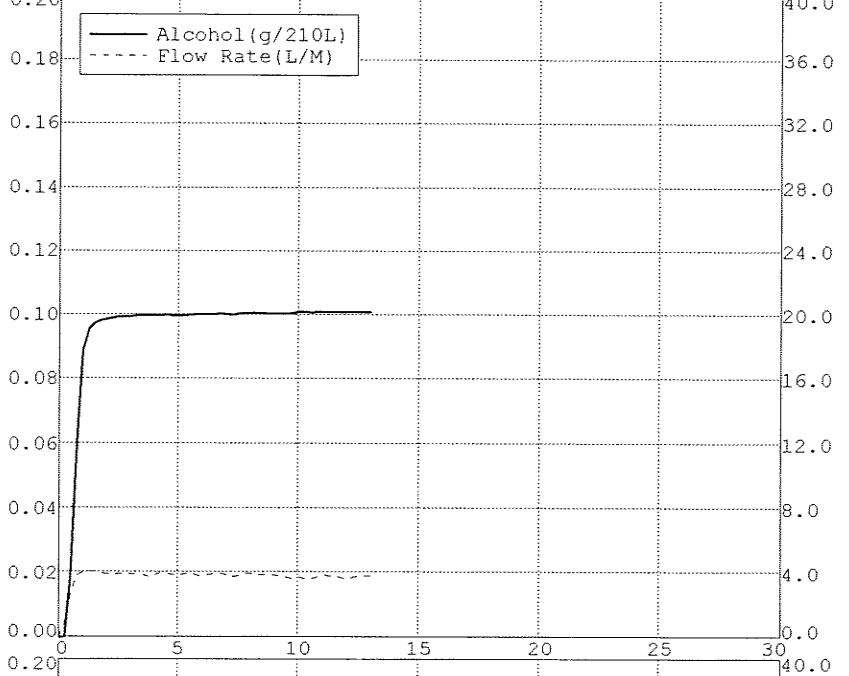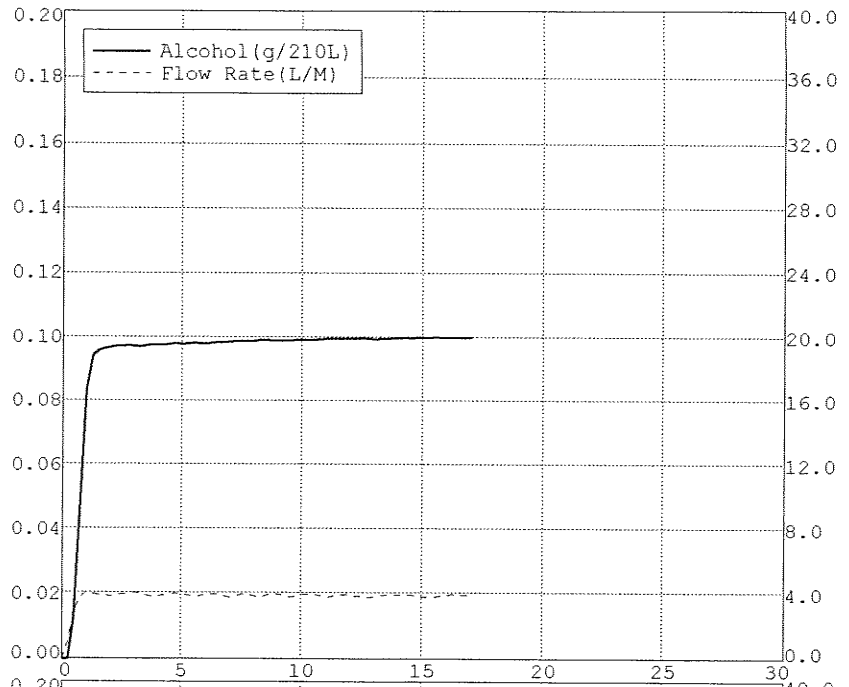

Charles B Geisler
[Signature]
#21170