

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 10/01/2021

OPERATOR NAME:
J RIEHL
Permit #: 47503
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:59
INTERNAL STANDARD	VERIFIED	00:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:59
BLANK TEST	0.00	01:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:00
BLANK TEST	0.00	01:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:01
BLANK TEST	0.00	01:02

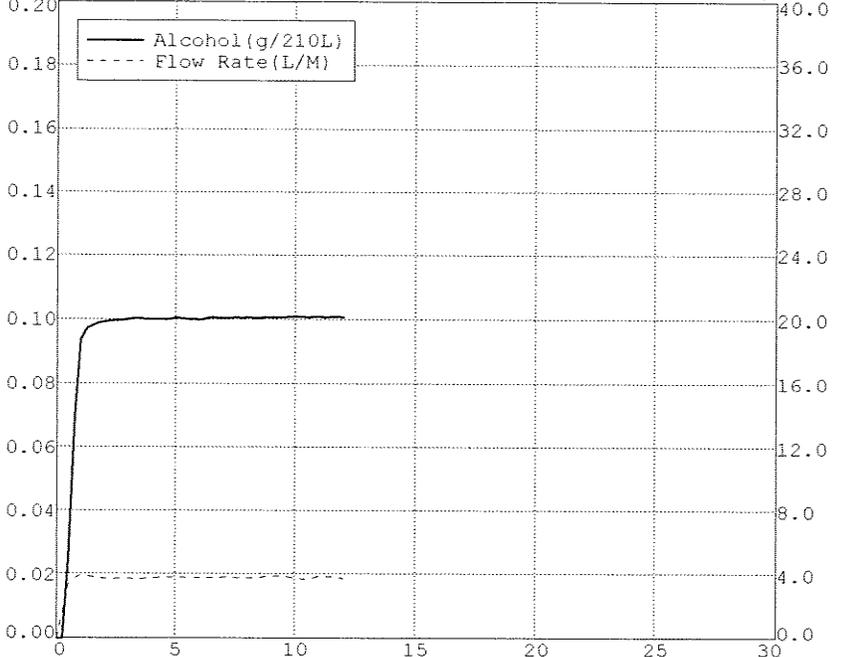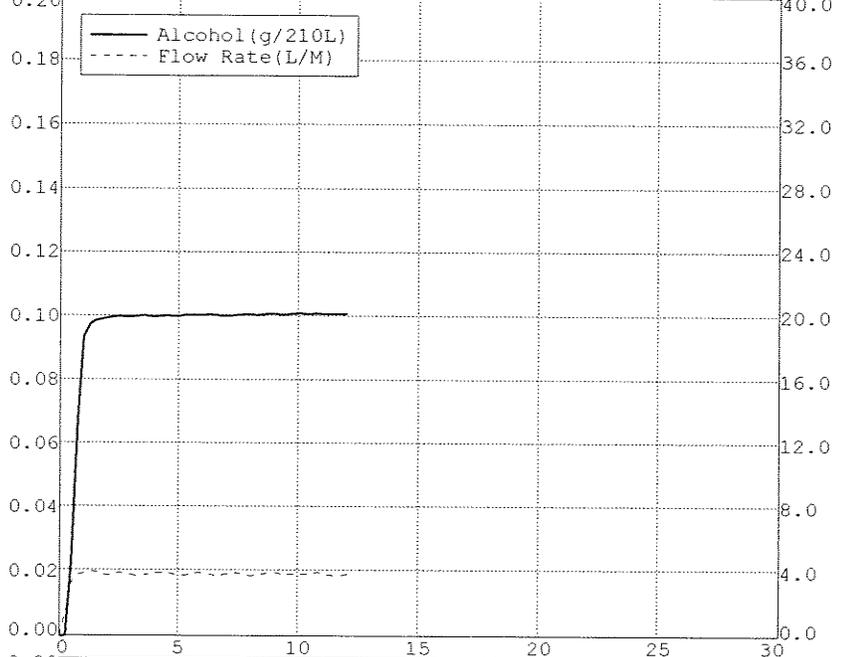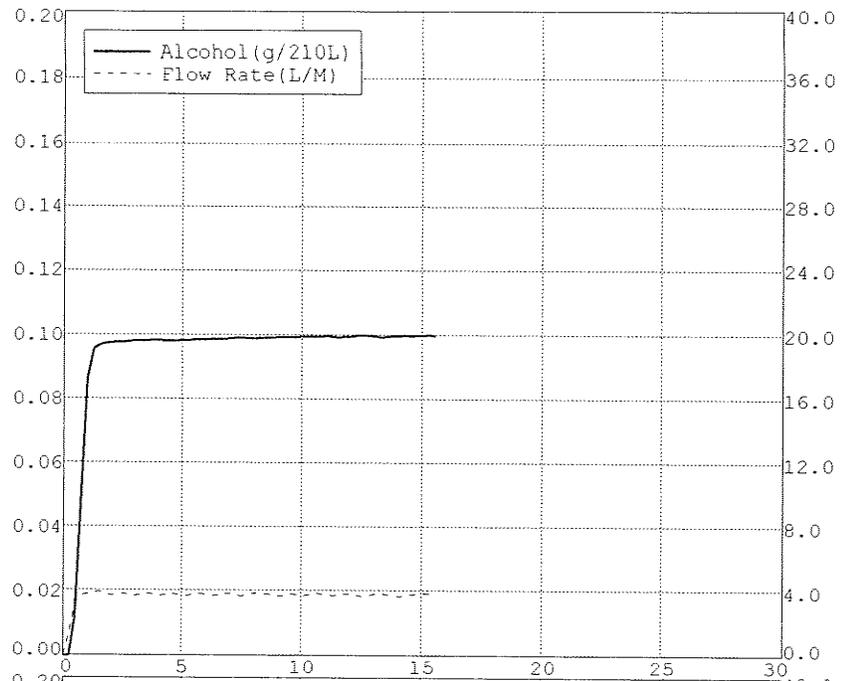

J Riehl
#820