

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/24/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:18
INTERNAL STANDARD	VERIFIED	12:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:19
BLANK TEST	0.00	12:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:20
BLANK TEST	0.00	12:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:21
BLANK TEST	0.00	12:22

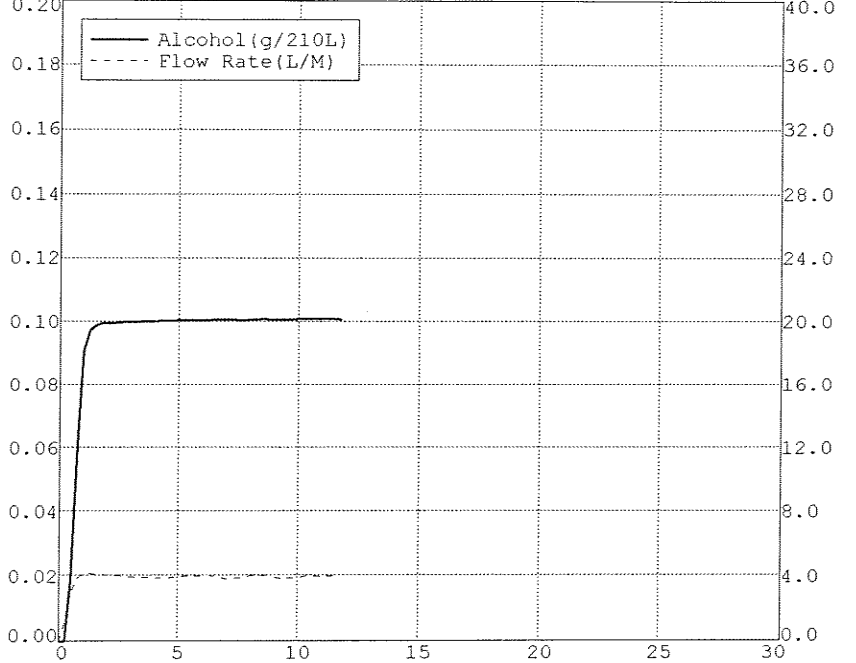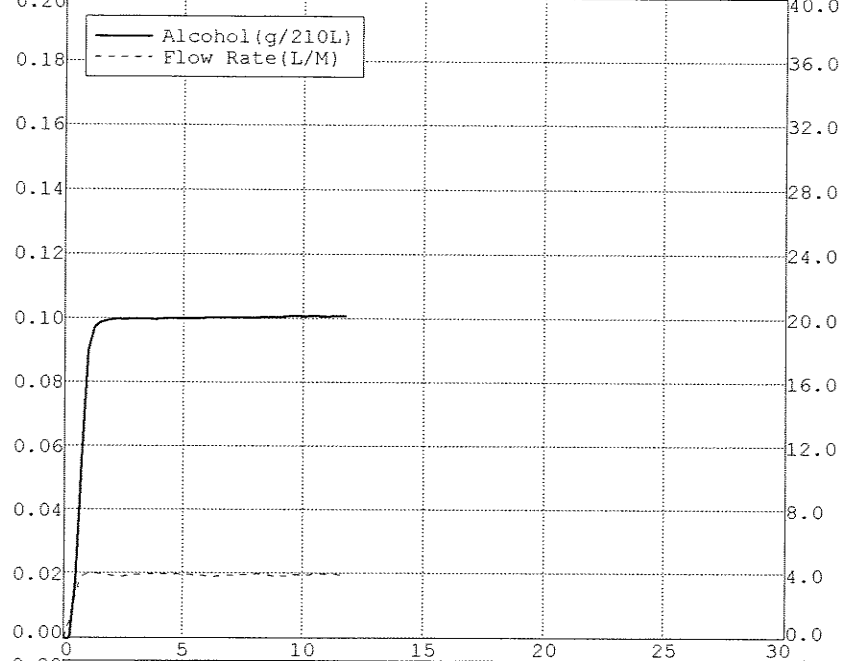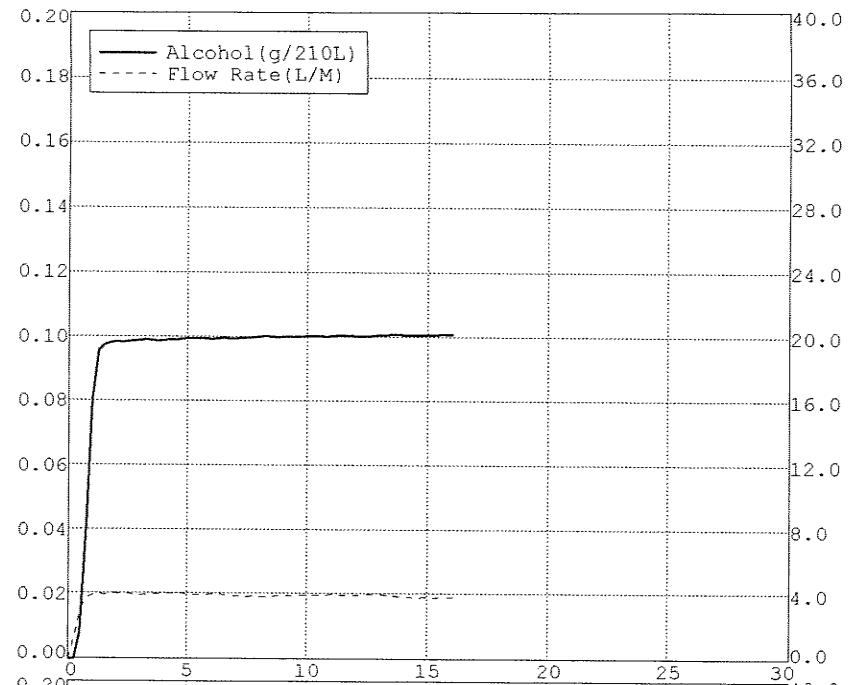

Charles B Geisler
#241