

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/17/2021

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:13
INTERNAL STANDARD	VERIFIED	09:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:14
BLANK TEST	0.00	09:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:15
BLANK TEST	0.00	09:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:16
BLANK TEST	0.00	09:17

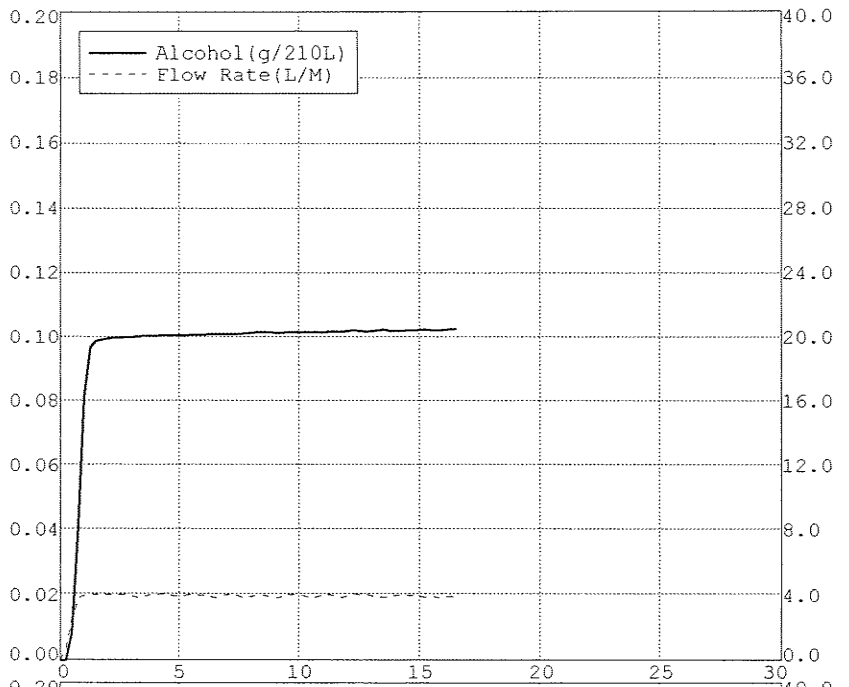

Handwritten signature and number 714