

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/01/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:45
INTERNAL STANDARD	VERIFIED	16:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:46
BLANK TEST	0.00	16:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:47
BLANK TEST	0.00	16:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:48
BLANK TEST	0.00	16:49

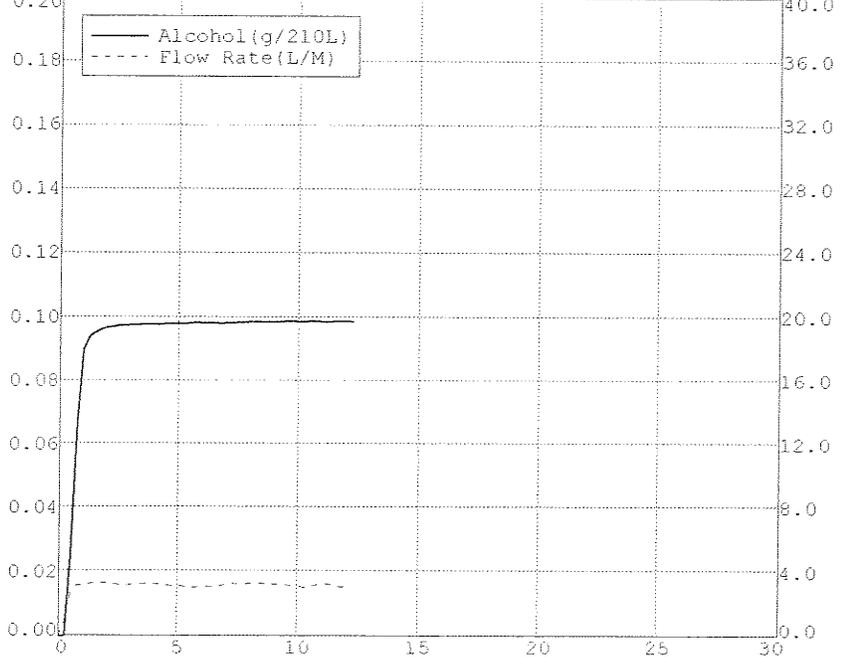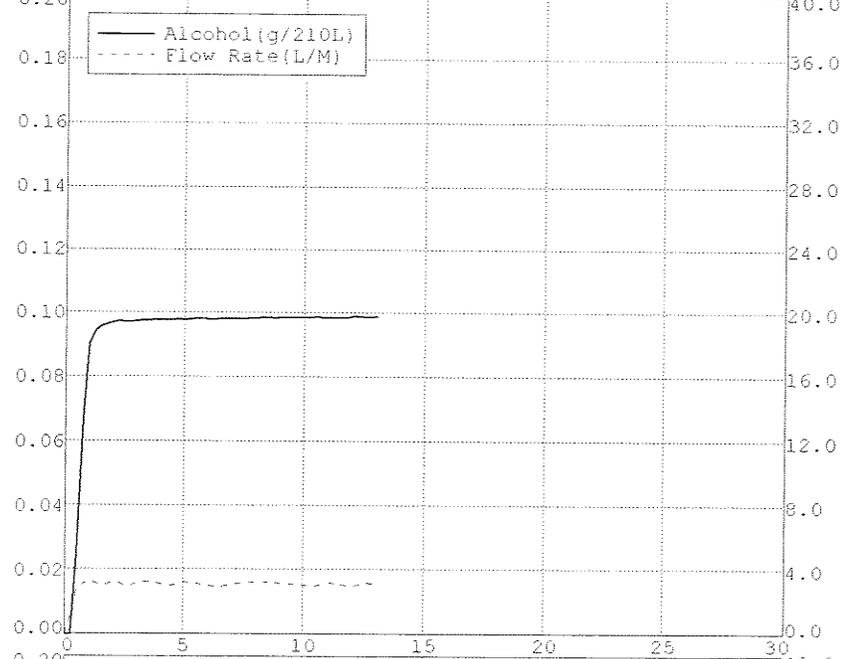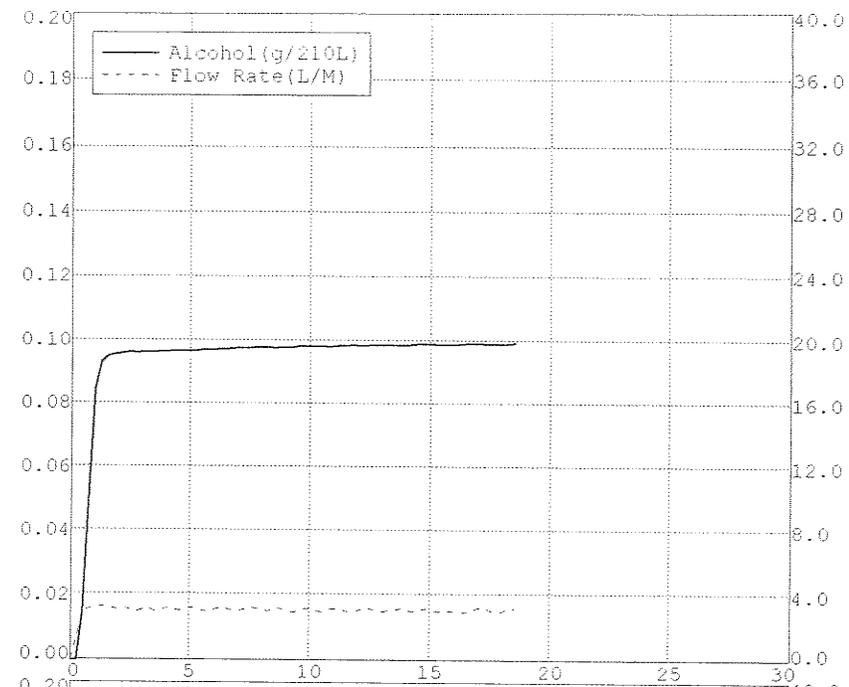

Charles B. Geisler