

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 01/07/2021

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:32
INTERNAL STANDARD	VERIFIED	15:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:33
BLANK TEST	0.00	15:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:35
BLANK TEST	0.00	15:36

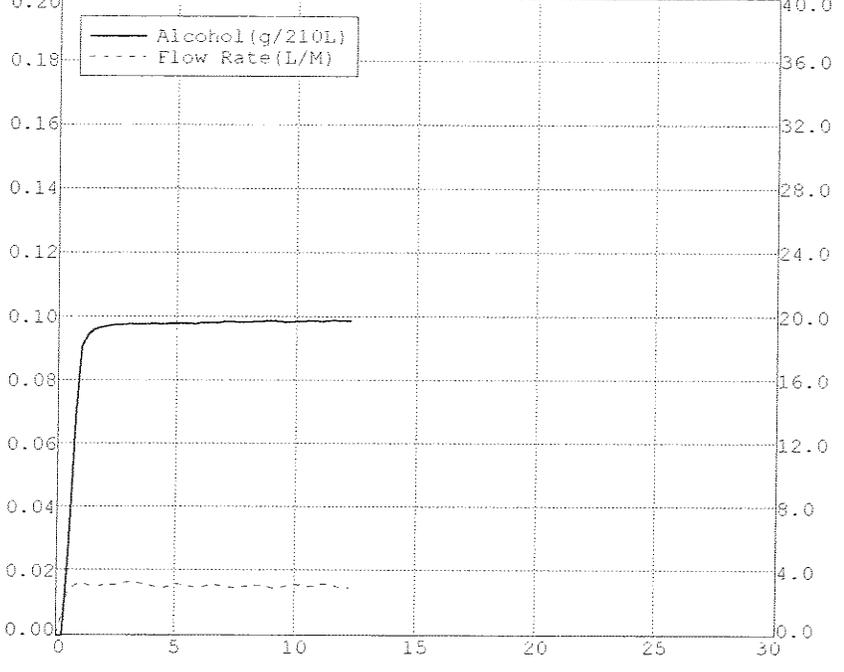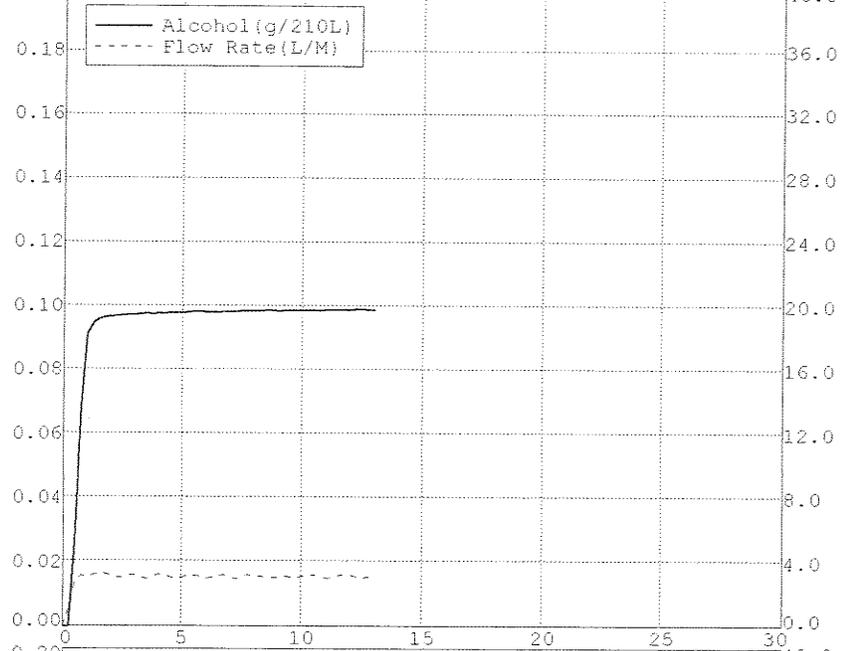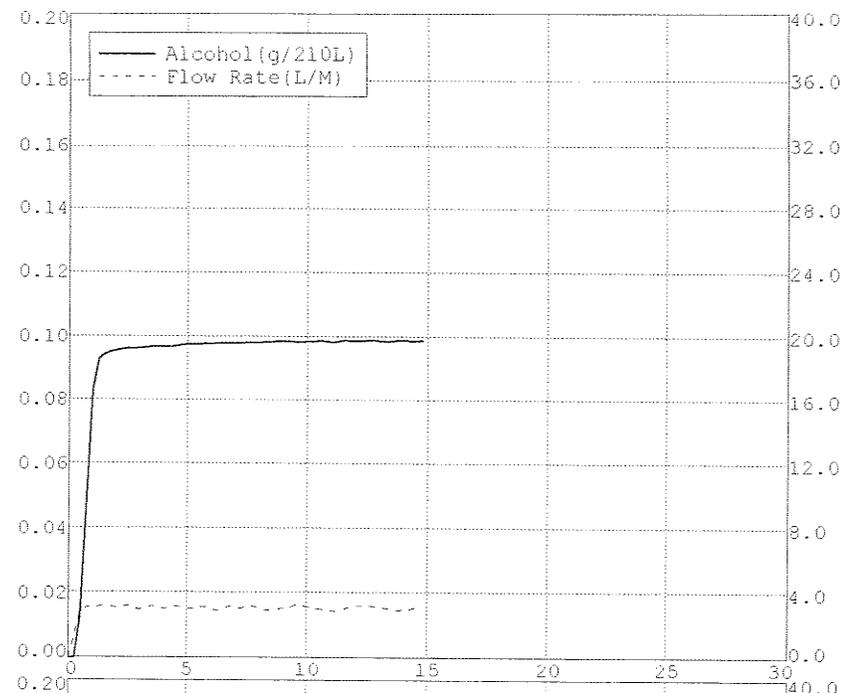

Handwritten signature and initials
 Sgt. [Signature] #2415