

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 01/29/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20430

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 17:45 |
| INTERNAL STANDARD       | VERIFIED | 17:45 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 17:45 |
| BLANK TEST              | 0.00     | 17:46 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 17:47 |
| BLANK TEST              | 0.00     | 17:47 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 17:48 |
| BLANK TEST              | 0.00     | 17:49 |

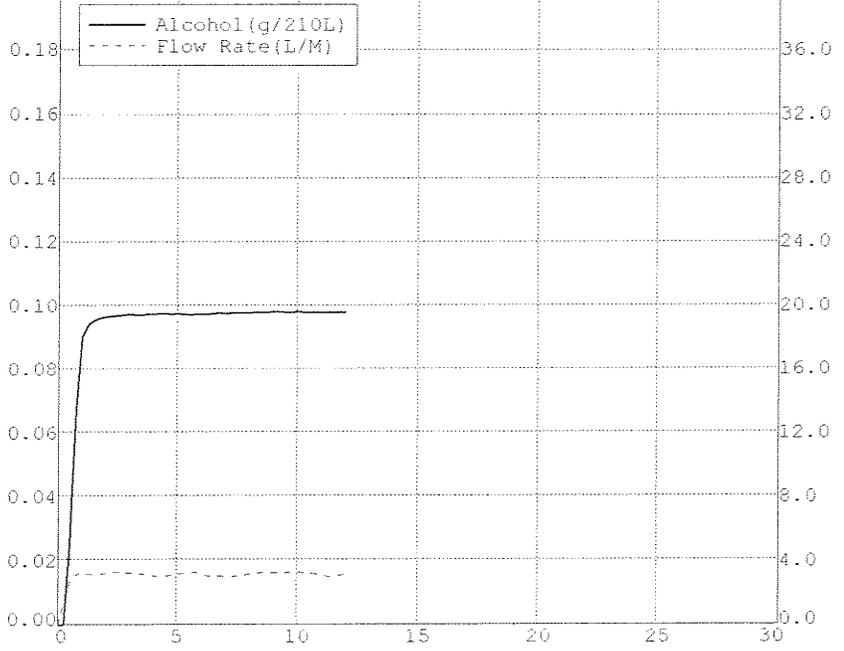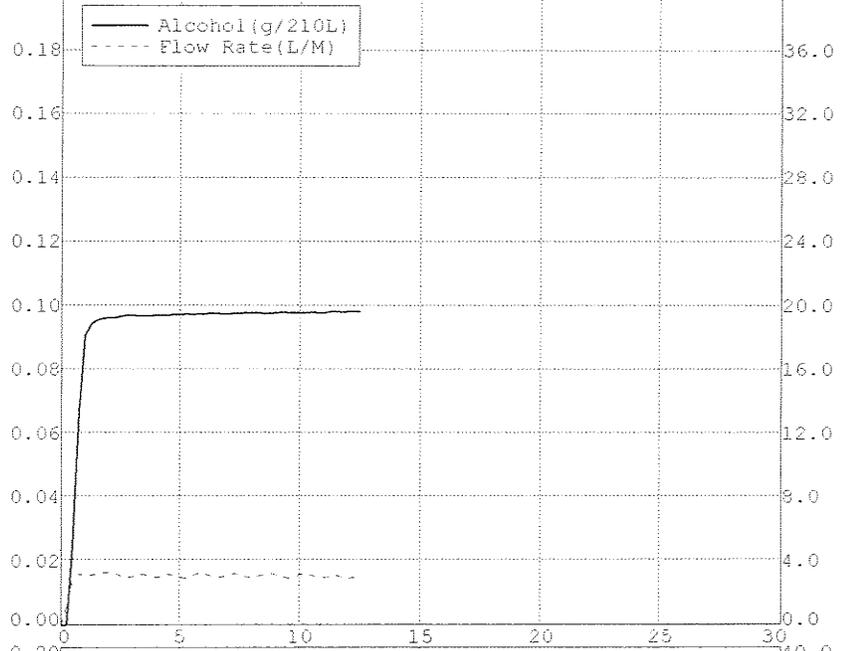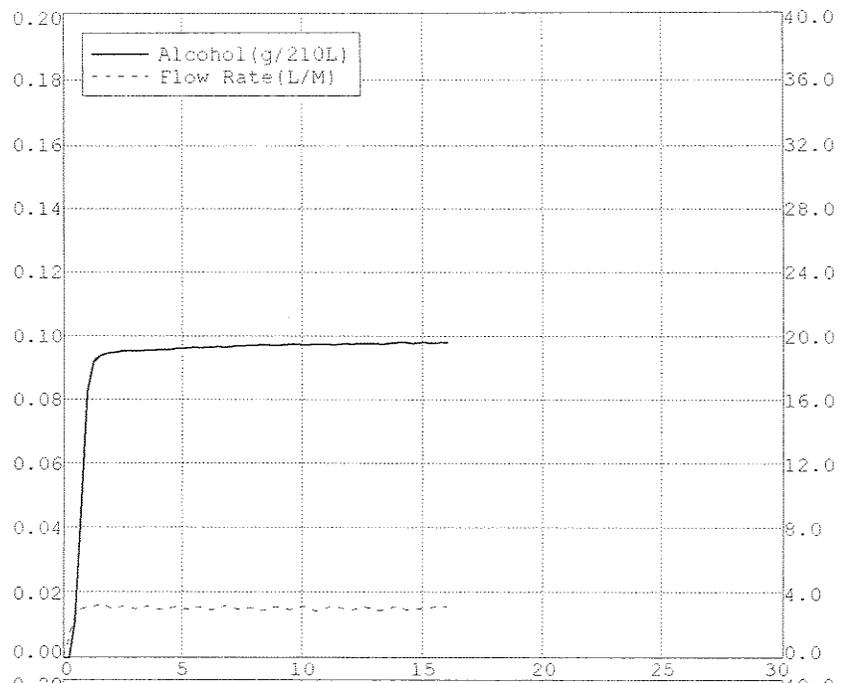

*Charles B. Geisler* #246