

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/08/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:57
INTERNAL STANDARD	VERIFIED	14:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:57
BLANK TEST	0.00	14:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:58
BLANK TEST	0.00	14:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:00
BLANK TEST	0.00	15:01

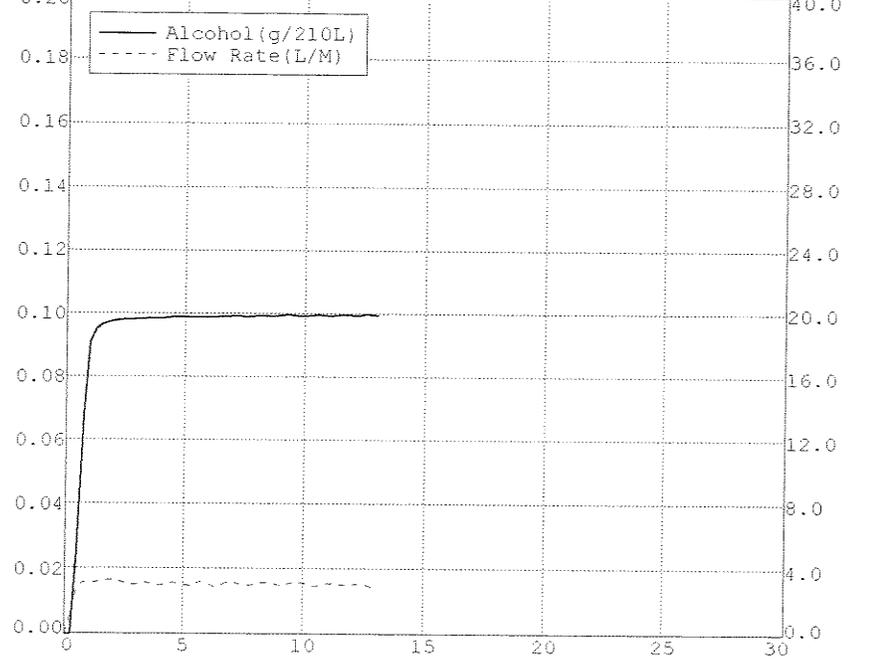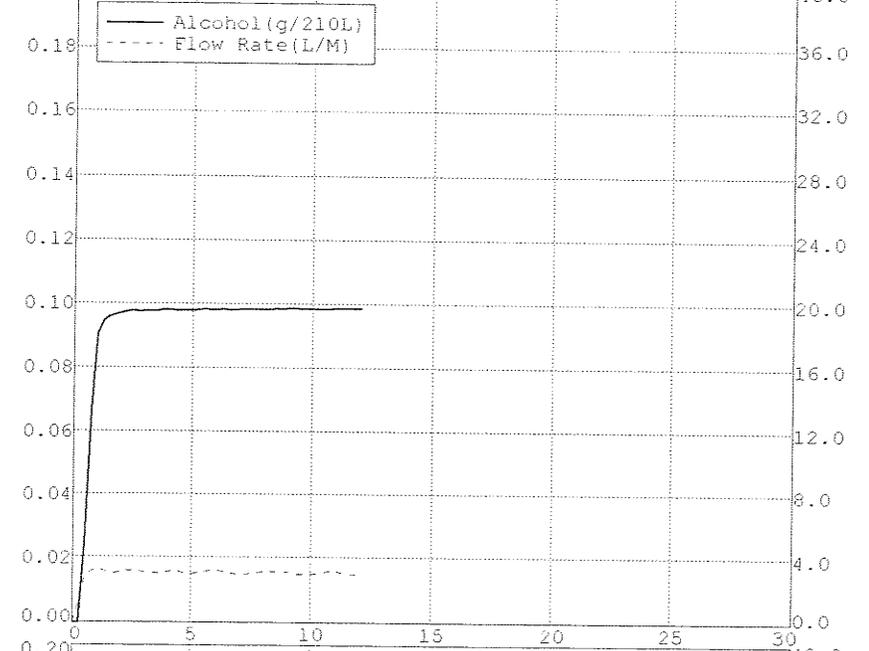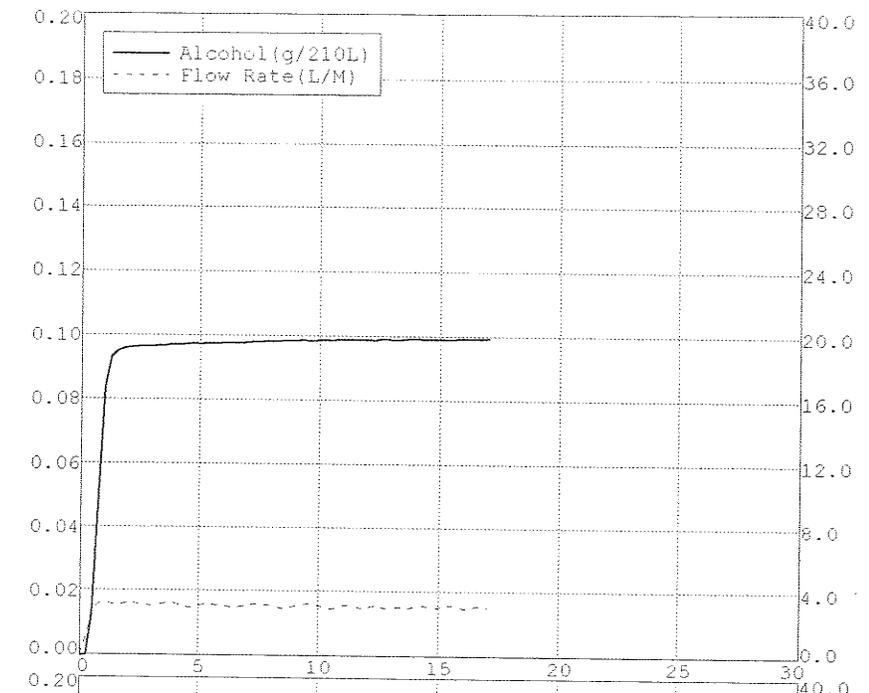

Handwritten signature and initials #241